


383

384 **Figure 6:** SFP displacement amplitudes in response to acoustic stimulation of the  
 385 tympanic membrane (~94 dB SPL) of ASTM [17] compliant temporal bones (n=10).  
 386 Black dashed lines represent the ASTM acceptance range and gray dashed lines  
 387 represent the extended acceptance range [14] used in this study.

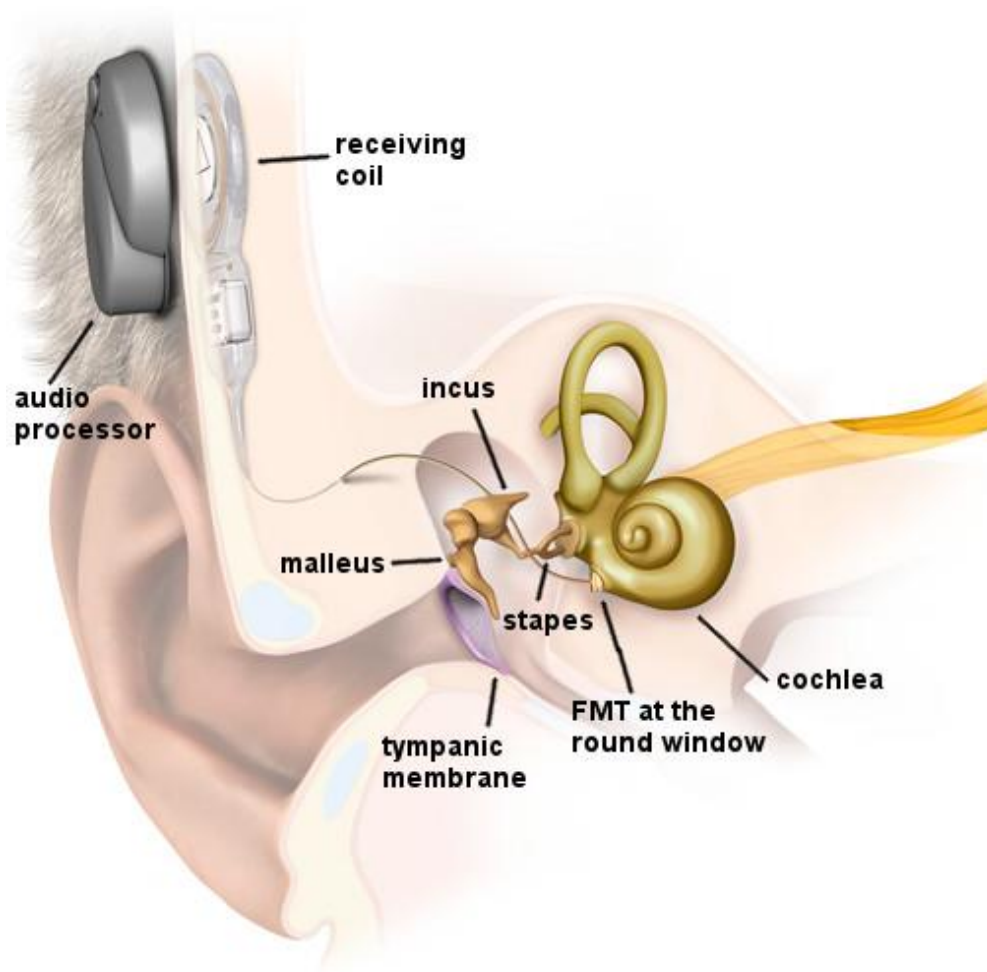

388

389 **Figure 7:** Schematic drawing of the human ear with implanted MED-EL Vibrant  
390 Soundbridge® when the Floating Mass Transducer (FMT) is placed at the round  
391 window of the cochlea.