

Automation of a Beckman liquid scintillation counter for data capture and data-base management

William Neil†, Thomas J. Irwin* and Joseph J. Yang

Mobil Environmental and Health Science Laboratory, P.O. Box 1029, Princeton, New Jersey 08540, USA

A software package for the automation of a Beckman LS9000 liquid scintillation counter is presented. The package provides effective on-line data capture (with a Perkin Elmer 3230 32-bit minicomputer), data-base management, audit trail and archiving facilities. Key features of the package are rapid and flexible data entry, background subtraction, half-life correction, ability to queue several sample sets pending scintillation counting, and formatted report generation. A brief discussion is given on the development of customized data processing programs.

^{14}C and ^3H radioisotopes have been frequently used in metabolism studies of drugs and other xenobiotics. They are also useful in comparing the relative absorption of a given compound from different routes of administration. Incorporation of either or both radioisotopes in the test compound allows for highly specific and sensitive determinations of the test compound and metabolites in the body tissues and excreta.

Liquid scintillation counting (LSC) is the method of choice in measuring such weak beta-emitting radioisotopes as ^3H and ^{14}C . The scintillation process involves interactions between a test sample containing beta emitters and the scintillation cocktail (a mixture of organic solvent and scintillator) leading to the emission of photons, which are measured by photomultiplier tubes in the LS counter.

Following a typical metabolism or bioavailability study in our laboratory, measurements of radioactivity in collected samples are effectively carried out with a Beckman LS9000 counter. It is equipped with three counting channels and with microprocessors that automatically correct for background and counting efficiency. However, the steps that follow which include data entry, record keeping, documentation, and quality assurance of numerous quantities of LSC data are laborious and time-consuming and in need of obvious automation.

Although LSC data capture software has been recently developed for use with laboratory personal computers

[1], the availability of data management and application software has been limited. A review of the commercially available software packages did not provide reasonable solutions to our needs in data capture, data-base management and data processing. Thus, we have chosen to develop our own LSC automation system (LSCAS) which includes the following principal features:

- (1) Automatic data capture—LSC data generated by the counter is captured on-line with a minicomputer.
- (2) Flexibility—unlimited selections are available for sample identification.
- (3) Reduction of record-keeping—data are clearly documented with proper sample identifications.
- (4) GLP requirements—data cannot be edited without specific documentation.
- (5) Efficient data management—data can be easily archived and retrieved.
- (6) Elimination of data entry—data generated from the counter are automatically entered into the customized application programs for data processing.

This paper delineates our efforts in the automation of data capture and data-base management. Details on the development of application programs to perform customized processing of LSC data will be published in a separate paper.

Materials and methods

Computer equipment

LSCAS consists of an Ergo CRT display terminal, a Perkin-Elmer 3230 32-bit minicomputer with a 300 megabyte disk, a Beckman LS9000 liquid scintillation counter equipped with a standard RS232 interface and a Perkin-Elmer CP100 printer. The Perkin-Elmer is linked to a VAX 11/750 using a VAX 3780 Protocol Emulator (Digital Equipment Corporation).

Computer software

The software package for LSCAS was written in FORT-RAN 77 under Perkin-Elmer OS32 operating system. There are five major components in the package: data collection, queue maintenance, status reports, archive maintenance and application programs.

† To whom correspondence and requests for reprints should be addressed.

* Present address: Squibb E. R. & Sons, Inc., Medical Affairs, P.O. Box 4000, Princeton, New Jersey 08540, USA.

<u>AVAILABLE PROGRAMS</u>			
1 - INSTRUMENT #: 01		1) BIOAVAILABILITY	
2 - PROGRAM #: 04	USER #: 04	2) IN VITRO PERCUTANEOUS ABSORPTION	
3 - STARTING POSITION #: 0020		3) HISTOGRAM GENERATION	
4 - ENDING POSITION #: 0034		4) OXIDIZER EFFICIENCY	
5 - DATE-OF-INITIATION: 11/11/11		5) LSC CALIBRATIONS	
6 - APPLICATION PROGRAM #: 01		6) WIPE TESTS	
7 - INITIALS: WN		7) BIODEGRADATION	
8 - DATE-OF-RUN:			
9 - DATE ARCHIVED:			

Figure 1. Sample scheduling data entry.

<u>SEQ#</u>	<u>POS#</u>	<u>ID#</u>	<u>SAMPLE DESCRIPTION</u>	<u>SAMPLE COMMENTS</u>	<u>BKGRD</u>	<u>#R</u>
001	020	010-111	BACKGROUND SAMPLE			01
002	021	010-111	BACKGROUND SAMPLE			02
003	022	010-111	BACKGROUND SAMPLE			03
004	023	010-112	FECES 24 HR		001-003	01
005	024	010-112	FECES 24 HR		001-003	02
006	025	010-112	FECES 24 HR		001-003	03
007	026	010-113	FECES 48 HR		001-003	01
008	027	010-113	FECES 48 HR		001-003	02
009	028	010-113	FECES 48 HR		001-003	03
010	029	010-112	URINE 24 HR		001-003	01
011	030	010-112	URINE 24 HR			02
012	031	010-113	URINE 24 HR	SAMPLE SLIGHTLY RED		01
013	032	010-113	URINE 24 HR	SAMPLE SLIGHTLY RED		02
014	033	010-111	URINE 48 HR			01
015	034	010-111	URINE 48 HR			02

Figure 2. Sample identification data entry. After the data in figure 1 has been entered, the user is provided with properly sequenced position numbers. Positive sample identification then occurs by entering the data that corresponds to its position in the liquid scintillation counter.

Data collection

Data entry

Procedures for entering sample identifications into LSCAS are divided into two parts as shown in figures 1 and 2. Three useful features were included into this portion of the program: (1) sequencing of sample position numbers occurs automatically as a result of the STARTING POSITION and ENDING POSITION parameters entered (figure 1). This saves the user from having to enter the position number for each individual sample; (2) SAMPLE COMMENTS (figure 2) can be used to describe sample characteristics and the generated records serve as an electronic notebook; and (3) automatic data entry is performed for replicates by entering the numerical value that corresponds to the number of replicates (# R in figure 2). Using triplicate as an example, information on the sample identification needs to be entered only for the first sample; identical information is automatically entered for two other samples.

A rapid and flexible data entry system is especially useful in LS counter automation. It is often desirable to add, delete or change descriptions from the menu. A pre-defined menu is extremely restrictive in a laboratory where changes are constantly being made on existing test procedures. An alternative of a free text entry for each sample provides flexibility but significantly increases the time required for data entry. Therefore, a second alternative was chosen which provides more efficiency. An unlimited number of user defined menus (figure 3) created using the text editor are implemented by entering a row of sample descriptions in the form of a template file. The program searches for the menu in the user's account providing a default menu in its absence.

The option to perform free text entries is still available by providing an additional selection (figure 3) DEFINE SITE, which will prompt the user for the sample description.

<u>SELECTION MENU</u>		
01) URINE 24 HR	15) FECES 120 HR	29) MUSCLE
02) URINE 48 HR	16) CAGE WASH	30) FAT
03) URINE 72 HR	17) HEART	31) BONE
04) URINE 96 HR	18) BRAIN	32) SKIN
05) URINE 120 HR	19) SMALL INTESTINE	33) RESIDUAL CARCASS
06) URINE WASH 24 HR	20) LARGE INTESTINE	34) SKIN WIPE
07) URINE WASH 28 HR	21) LIVER	35) CHARCOAL TUBE
08) URINE WASH 72 HR	22) KIDNEY	36) CELL
09) URINE WASH 96 HR	23) SPLEEN	37) TAPE
10) URINE WASH 120 HR	24) STOMACH	38) BLOOD
11) FECES 24 HR	25) TESTES	39) FETUS
12) FECES 48 HR	26) OVARIES	40) PLACENTA
13) FECES 72 HR	27) BLADDER	41) DOSE
14) FECES 96 HR	28) LUNG	42) CO2 TRAP SOLUTION
		43) PIPET RINSE
		44) SPATULA RINSE
		45) DEFINE SITE

ENTER ITEM NUMBER : ___

Figure 3. Sample selection menu. The number of sample description selections are unlimited due to the user-defined selection menus. Free text entry is also provided (option 45).

Data capture

The most vital section of LSCAS is its data capture program. Radioactivity values generated from the counter must be correctly matched with the corresponding sample identifications. Figure 4 graphically illustrates the algorithm that performs this function.

Basically, the LSC process is performed in the following fashion. Vials containing test samples and scintillation cocktail are placed in consecutive order into the counter in a sample conveyer train. Each sample has a specific position number corresponding to its location in the train. In the position immediately preceding the first vial of each sample set is a COMMAND TOWER. The

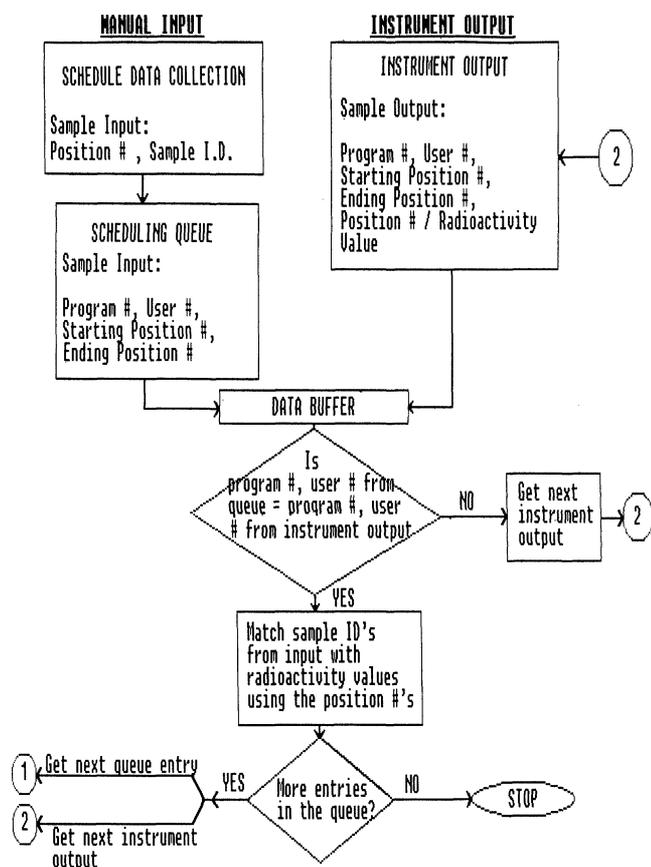


Figure 4. Flowchart of data capture process.

COMMAND TOWER contains four dials corresponding to the numbers 1, 2, 4, and 8. By dialling the appropriate combination of numbers, the user can select up to 10 counting programs (for example dialling 1, 3, and 4 selects program 8). The COMMAND TOWER is read by a photoelectric cell and instructs the counter what LSC program will be used for subsequent countings (for example isotope(s) counted, counting time). Only one COMMAND TOWER needs to be used if all samples are to be counted under the same program. A STOP TOWER (no dial settings) is placed directly after the last sample in the train to terminate the counting. All LSC data generated are sent via the RS232 interface to the Perkin-Elmer 3230 minicomputer where the matching of radioactivity values with sample identifications takes place.

Background subtraction

Radiation originating from the sample vial, the scintillation cocktail, or instrumental sources can result in low level background counts. These counts must be subtracted from the sample count, especially when analysing samples with minute amounts of radioactivity. Although the Beckman LS9000 counter allows a fixed background value to be subtracted from the LSC data of samples analysed, it is more desirable to perform background subtractions based on values obtained from sample blanks prepared specifically for the corresponding sets of samples. In LSCAS, this latter approach is accomplished by placing the sample blanks in consecutive order into the

sample conveyer train and supplying the program with the position number of sample blanks (figure 2).

Half-life corrections

LSC of radioisotopes, especially those with short half-life (for example ^{32}P , ^{125}I), requires correction factors due to loss of inherent radioactivity through decay. Half-life corrections are easily performed on late model LS counters by supplying the counter with information on the time lag between a specified date and the analysis date. This feature is not available on the Beckman LS9000 counter, therefore a separate step has been included in LSCAS to perform similar automatic half-life corrections.

Data documentation

In order to meet requirements of Good Laboratory Practices (GLP), LSCAS was designed with an AUDIT TRAIL feature which documents any changes made to the raw data regarding who, what, where, when and how. In LSCAS, a user cannot modify any radioactivity data generated originally by the counter but can change entries such as sample identification number provided that appropriate reasons are given. The AUDIT TRAIL file can be examined at any time as shown in figure 5.

AUDIT TRAIL FOR FILE #F84JR5.DAT

DATE	INITIALS	CODE	REASON
01/25/86	WN	0	ENTERED INCORRECT PROJECT # PROJECT #50101 WAS CHANGED TO #51011
01/25/86	WN	0	ENTERED INCORRECT ID # POSITION #125 ID #000-101 WAS CHANGED TO ID #000-102

Figure 5. Typical Audit trail file.

The raw data in LSCAS are also protected with the following measures: (1) each sample data set is assigned a unique data file name and the data file is placed into a protected account, separate from the user's account, to prohibit editing by the user. (2) Users are not allowed to access the LSC data from another user's account. This is accomplished by searching through a master data file (containing the file history of all collected sample sets) for the account number under which the data was saved. This account number must match the account number of the user currently seeking to access the data.

Queue maintenance

QUEUE MAINTENANCE allows sample data sets to be placed on a 'waiting list' (queue) in LSCAS pending LSC counting. After scheduling the sample sets to be counted under data collection, they must then be placed into the queue. Each entry into the queue represents a sample data set under one COMMAND TOWER and as a result, the user does not need to individually start the automation process for each sample data set. This setup is extremely useful when counting sets of samples overnight allowing the (automation) process to operate continuously.



Hindawi

Submit your manuscripts at
<http://www.hindawi.com>

