

Research Article

Biomechanical Comparison of Multilevel Lumbar Instrumented Fusions in Adult Spinal Deformity According to the Upper and Lower Fusion Levels: A Finite Element Analysis

Dong-Min Son,¹ Soo-Bin Lee²,³ Sung-Jae Lee,¹ Tae-Hyun Park,¹ Ji Eun Jang,³ Seung Jo Jeong,³ Young-Mi Kang,⁴ and Byung Ho Lee⁴

¹Department of Biomedical Engineering, College of Biomedical Science & Engineering, Inje University, 197 Inje-ro, Gimhae-si Gyeongsangnam-do 50834, Republic of Korea

²Department of Orthopedic Surgery, Catholic Kwandong University International St. Mary's Hospital, 25, Simgok-ro 100beon-gil, Seo-gu, Incheon 22711, Republic of Korea

³GS Medical Co., Ltd., 90 Osongsaengmyeong 4-ro, Osong-eup, Heungdeok-gu, Cheongju-si, Chungcheongbuk-do 28161, Republic of Korea

⁴Department of Orthopedic Surgery, Yonsei University College of Medicine, 50 Yonsei-ro, Seodaemun-gu, Seoul 03722, Republic of Korea

Correspondence should be addressed to Byung Ho Lee; bhlee96@yuhs.ac

Dong-Min Son and Soo-Bin Lee contributed equally to this work.

Received 20 July 2022; Revised 11 November 2022; Accepted 14 November 2022; Published 30 November 2022

Academic Editor: Panagiotis Korovessis

Copyright © 2022 Dong-Min Son et al. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Multilevel lumbar fusion with posterior pedicle screw fixation is a widely performed surgical procedure for the management of adult spinal deformity. However, there has not been a comprehensive biomechanical study on the different types of fusion levels in terms of stability and possible complications. We aimed to investigate the biomechanical properties of multilevel lumbar fusion according to different types of upper and lower fusion levels. Six different types of fusions were performed using three-dimensional finite element models. Type A and B referred to the group of which upper fusion level was L1 and T10, respectively. Subtype 1, 2, and 3 referred to the group of which lower fusion level was L5, S1, and ilium, respectively (A1, L1-L5; A2, L1-S1; A3, L1-ilium; B1, T10-L5; B2, T10-S1; B3, T10-ilium). Flexion, extension, axial rotation, and lateral bending moments were applied, and the risk of screw loosening and failure and adjacent segment degeneration (ASD) was analyzed. Stress at the bone-screw interface of type B3 was lowest in overall motions. The risk of screw failure showed increasing pattern as the upper and lower levels extended in all motions. Proximal range of motion (ROM) increased as the lower fusion level changed from L5 to S1 and the ilium. For axial rotation, type B3 showed higher proximal ROM (16.2°) than type A3 (11.8°). In multilevel lumbar fusion surgery for adult spinal deformity, adding iliac screws and increasing the fusion level to T10-ilium may lower the risk of screw loosening. In terms of screw failure and proximal ASD, however, T10-ilium fusion has a higher potential risk compared with other fusion types. These results will contribute for surgeons to provide adequate patient education regarding screw failure and proximal ASD, when performing multilevel lumbar fusion.

1. Introduction

Multilevel lumbar fusion with posterior pedicle screw fixation is a widely performed surgical procedure for the management of adult spinal deformity [1]. As global life expectancy is con-

tinuously increasing, and due to the development of medical care, the incidence and prevalence of adult spinal deformity are on the rise [2–4]. Previously, conservative management was recommended owing to higher morbidity associated with surgery [2]; however, surgical intervention with multilevel

lumbar fusion has become the mainstay of adult spinal deformity treatment recently [4]. Numerous literatures have reported the superiority of multilevel lumbar fusion for the treatment of various types of adult spinal deformity [1, 5–9].

Multilevel lumbar fusion surgery has the advantage of spinal alignment correction; however, complications such as screw breakage and loosening or adjacent segment degeneration may occur. To avoid these complications associated with lumbar fusion surgery, artificial disc replacement (ADR) was developed for degenerative lumbar spinal diseases which do not require alignment correction. In a study using finite element analysis, single level ADR showed satisfactory results; however, multilevel ADR showed hypermobility which may lead to alter natural movement of spine and implant failure [10]. In clinical practice, whether ADR is superior to fusion is still controversial. To date, there is no other alternative than multilevel fusion surgery for adult spinal deformities requiring spinal alignment correction.

However, to our knowledge, there has not been a comprehensive biomechanical study on the different types of fusion levels in terms of stability and possible complications. Most previous studies were confined to complications about L5-S1 segment or proximal adjacent segment [11–14]. Furthermore, most studies on multilevel lumbar fusion were cadaveric experiments or clinical observational studies with a small sample size [13, 15, 16]. In this study, we aimed to investigate the biomechanical properties of multilevel lumbar fusion according to the different types of upper and lower fusion levels.

Using finite element analysis, we therefore asked: (1) How different is the risk of screw loosening between the fusion types? (2) How different is the risk of screw failure between the fusion types? (3) How different is the risk of adjacent segment degeneration (ASD) between the fusion types?

2. Materials and Methods

Ethical approval for this study was obtained from the Institutional Review Board (IRB) of the corresponding author's hospital (Yonsei University IRB and Ethics Committee: 4-2020-0060). All methods were performed in accordance with the Declaration of Helsinki and Yonsei University institutional guidelines. Informed consent was obtained from the subject.

2.1. Finite Element Analysis of an Intact Thoracolumbar Spine and Pelvis Model. A three-dimensional (3D) thoracolumbar spine and pelvis model was constructed using computed tomography data from a normal 57-year-old male, with the slice thickness of 2-mm, along with a previously validated lumbar spine model called T9-Pelvis (Figure 1) [17]. All model moieties were created using 0.3 mm tetrahedral mesh. The mesh convergence in the present study was decided among varying element sizes. With an element size of 0.3 mm, the stress converged properly. Finally, a 0.3 mm element size was applied in our study. The finite element model consisted of the thoracolumbar and pelvic bone, intervertebral disc, and major ligaments. The number of

nodes was 250,495, and the number of elements was 1,307,709 for the intact model.

We used Abaqus (version 6.14; Dassault Systems, France) to perform finite element analysis and computer-aided engineering of the spine model. We constructed the thoracolumbar spine ligaments as a truss element including the anterior longitudinal ligament, posterior longitudinal ligament, ligamentum flavum, intertransverse ligament, interspinous ligament, supraspinous ligament, and capsular ligament. We constructed the pelvic ligaments as a spring including the anterior sacroiliac ligament, posterior sacroiliac ligament, interosseous sacroiliac ligament, sacrospinous ligament, sacrotuberous ligament, superior pubic ligament, arcuate ligament, inguinal ligament, and iliolumbar ligament. The Young's modulus, Poisson's ratio, and stiffness coefficient were applied to each moiety using previously published data in the literature (Tables 1 and 2) [18–23].

We used two methods to validate the finite element analysis results. (1) The lumbar lordosis angle of the 3D model was measured and compared with the angle in the normal range [24]. (2) The range of motion (ROM) of the thoracic spine was measured by applying a pure moment (7.5 Nm) suitable for spinal mobility, and the results were compared with those in the literature [25, 26].

2.2. Finite Element Analysis of Surgical Models. We produced the surgical model by importing the oblique lateral interbody fusion (OLIF) and posterior lumbar interbody fusion (PLIF) cage (GS Medical, Osong, Korea) into Abaqus. The OLIF/PLIF cage dimensions were 22 mm/26 mm in length, 22 mm/14 mm in height, and 12°/6° in angle measure, respectively, according to the lumbar model height and angle. The discs of each intact lumbar segment were removed; OLIF cages were inserted into L1-L5, and PLIF cages were inserted into L5-S1. The pedicle screw system (GS Medical) was used for posterior fixation: 6.5 mm in diameter and 45 mm in length for the spine and 8.5 mm in diameter and 80 mm in length for the ilium. The pedicle screw was inserted through the center of the pedicle and parallel to the endplate, and the iliac screw was inserted through S2 ala (S2 alar-iliac screw) [27]. Next, a 6.0 mm diameter rod was constructed and attached according to the position of the pedicle screw housing. The following material properties of Grade 5 titanium (Ti-6Al-4V) were used for the model analysis: Young's modulus = 110,000 MPa; Poisson's ratio = 0.35 [28].

Six different fusion types for comparative analysis were made. Type A and B referred to the group of which upper fusion level was L1 and T10, respectively. Subtype 1, 2, and 3 referred to the group of which lower fusion level was L5, S1, and ilium, respectively: Type A1, L1-L5; Type A2, L1-S1; Type A3, L1-iliac; Type B1, T10-L5; Type B2, T10-S1; Type B3, T10-iliac (Figure 2).

2.3. Loading and Boundary Conditions. To apply a physiological load, both acetabulum bones were fixed in all degrees of freedom, assuming standing on two legs. A pure moment of 10 Nm was applied to the uppermost segment (T9) endplate in the direction of flexion, extension, axial rotation,

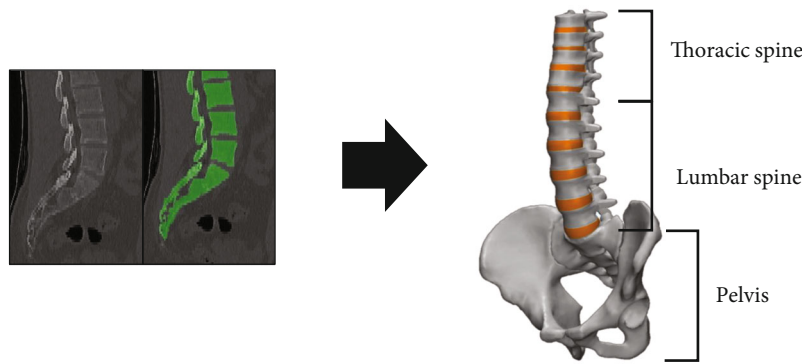


FIGURE 1: Construction of a 3-dimensional spine model using computed tomography data.

TABLE 1: Material properties of the spine.

| Materials | Young's modulus (Mpa) | Poisson's ratio |
|-----------------------------|-----------------------|-----------------|
| Ilium (cortical) | 17,000 | 0.3 |
| Ilium (cancellous) | 132 | 0.2 |
| Sacrum (cortical) | 6140 | 0.3 |
| Sacrum (cancellous) | 1400 | 0.3 |
| Vertebral body (cortical) | 12,000 | 0.3 |
| Vertebral body (cancellous) | 100 | 0.3 |
| Posterior elements | 3500 | 0.25 |
| Annulus fiber | 450 | |
| Annulus matrix | 4.2 | 0.45 |
| Nucleus pulposus | 1 | 0.499 |
| Endplate | 100 | 0.3 |

TABLE 2: Material properties of the pelvic ligaments.

| Materials | Stiffness coefficient (N/mm) |
|---------------------------------------|------------------------------|
| Anterior sacroiliac ligament | 700 |
| Posterior sacroiliac ligament (long) | 1000 |
| Posterior sacroiliac ligament (short) | 400 |
| Interosseous sacroiliac ligament | 2800 |
| Sacrospinous ligament | 1400 |
| Sacrospinous ligament | 1500 |
| Superior pubic ligament | 500 |
| Arcuate pubic ligament | 500 |
| Inguinal ligament | 250 |
| Iliolumbar ligament | 1000 |

and lateral bending according to the spinal mobility. A compressive follower load of 400 N was applied according to the curvature of the vertebral segment (Figure 3) [29]. Tie contact conditions were applied assuming that the bone-implant and implant-implant interfaces were completely fused and fixed. Since the size of the finite element model was large, we tried to simplify it and show the potential risk

of screw loosening using analysis of the stress occurring in the screw-bone interface.

3. Results

3.1. Peak Von Mises Stress at the Bone-Screw Interface. Stress at the bone-screw interface of type B3 was lowest in overall motions. Subtype 2 showed higher peak von Mises stress (PVMS) than subtype 1 and 3. For flexion and extension, subtype 1 and 3 showed similar results within type A and B group while type A showed higher PVMS than type B. For axial rotation, type B1 showed higher PVMS than B3. PVMS was noted at the upper end level in subtype 3 and axial rotation motion in all types, while PVMS was noted at the lower end level in other types and motions (Figure 4).

3.2. Peak Von Mises Stress at the Screw. PVMS at the screw increased as the lower fusion level changed from L5 to S1 and the ilium. Type B group showed slightly higher results in all motions than the type A group. The highest PVMS was identified in axial rotation motion, and type B3 showed the highest PVMS (267.8 MPa) among the six types. The measured stress in all motion and types was less than the yield strength (880 MPa) of Grade 5 titanium (Ti-6Al-4 V) (Figure 5). Among all the types, the highest PVMS occurred at the neck of the lowest screw in flexion and extension and at the neck of uppermost screw in lateral bending. In axial rotation, the highest PVMS occurred at the neck of L4 screw in type A group and at the neck of T12 screw in type B group (Figure 6).

3.3. Range of Motion at Adjacent Segments. Overall, the proximal ROM increased as the lower fusion level changed from L5 to S1 and the ilium. For flexion, extension, and lateral bending, type B group showed similar or slightly higher proximal ROM than each corresponding type A. For axial rotation, type B3 showed higher proximal ROM (16.2°) than type A3 (11.8°). Despite interbody fusion with two cages in the L5-S1 segment, fine motion in L5-S1 was identified in subtype 2 group, whereas subtype 3 group showed no motion (Figure 7).

4. Discussion

Advantages of multilevel lumbar fusion with posterior pedicle screw fixation have been reported in numerous studies,

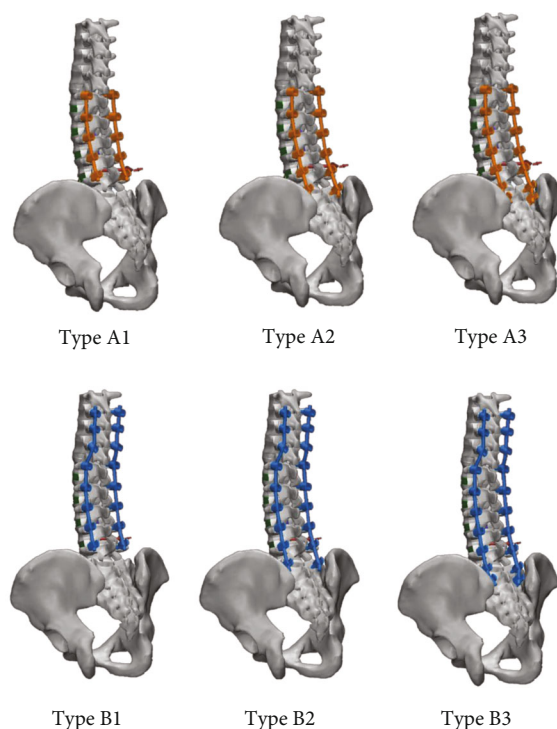


FIGURE 2: Construction of six different surgical model types for comparative analysis of the fusion level: Type A1, L1-L5 fusion; Type A2, L1-S1 fusion; Type A3, L1-iliac fusion; Type B1, T10-L5 fusion; Type B2, T10-S1 fusion; Type B3, T10-iliac fusion.

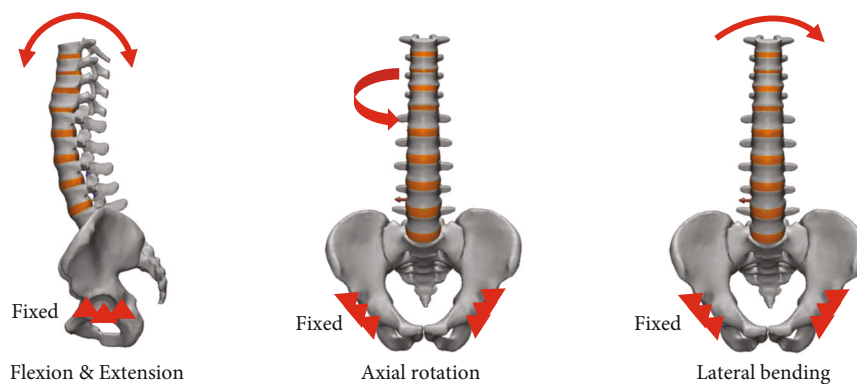


FIGURE 3: Application of a physiological load to the spine model.

and possible complications also have been researched using various methods. However, to our knowledge, there has not been a comprehensive study on biomechanical properties of different fusion levels using 3-dimensional finite element method. We found that adding iliac screws and increasing the fusion level to T10-iliac may lower the risk of screw loosening. Second, in terms of screw failure and proximal ASD, T10-iliac fusion model showed higher potential risk compared with other fusion types. Based on these results, it can be suggested that T10-iliac fusion is recommendable for spinal deformity correction and maintaining the stability, although there is a potential risk of screw failure and proximal ASD; therefore, surgeons should provide adequate patient education regarding screw failure and proximal ASD, when performing T10-iliac fusion.

In terms of screw loosening, we found that type B3 was most appropriate in overall motions. The stress at the bone-screw interface in fusion down to S1 is 58% higher on average than that in fusion down to L5 or the iliac regardless of the upper fusion level. This result was consistent with previous literature findings [30–33]. Also, type A group showed 61% higher PVMS on average than type B group in flexion and extension, possibly due to high loading at the remaining mobile T12-L1 segment. In axial rotation, type B3 showed 28% superior result compared with type B1, indicating the strong fixation effect of axial movement by iliac screws (Figure 4). The use of iliac screw has been shown to improve biomechanical stability. Yasuda et al. reported various complications including loosening, 76% in noniliac fusion group and 12% in iliac fusion group [34].

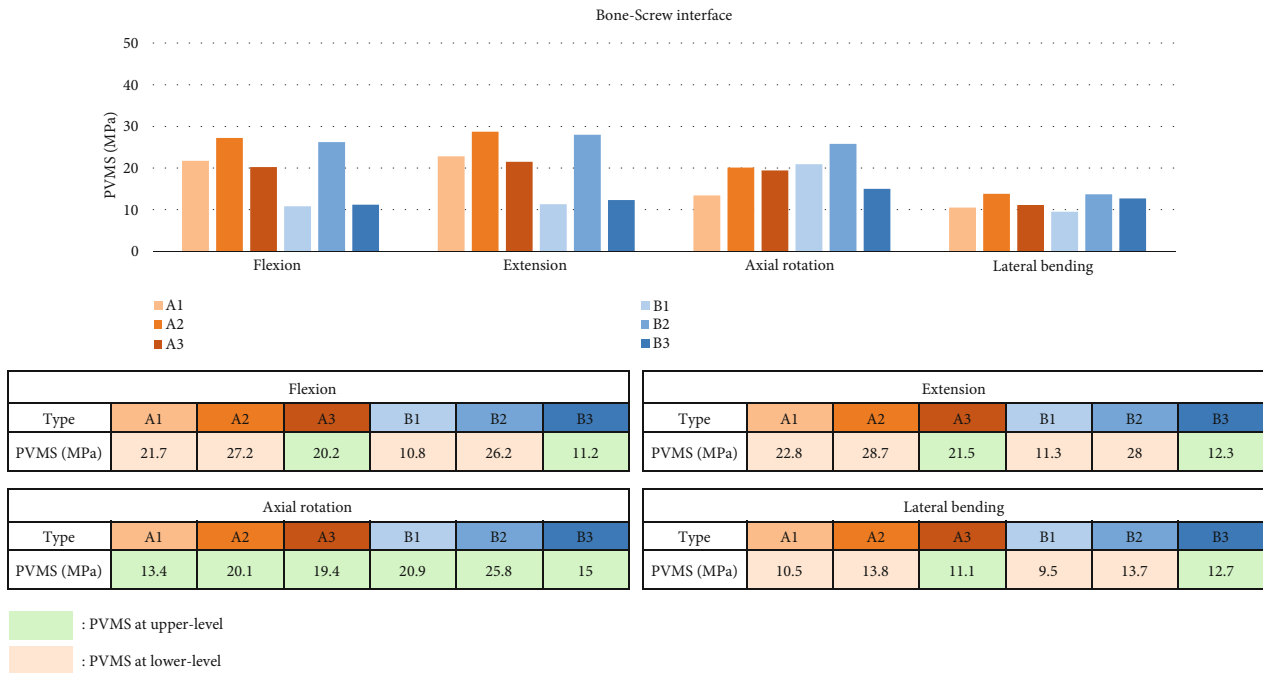


FIGURE 4: Peak von Mises stress measured at the bone-screw interface.

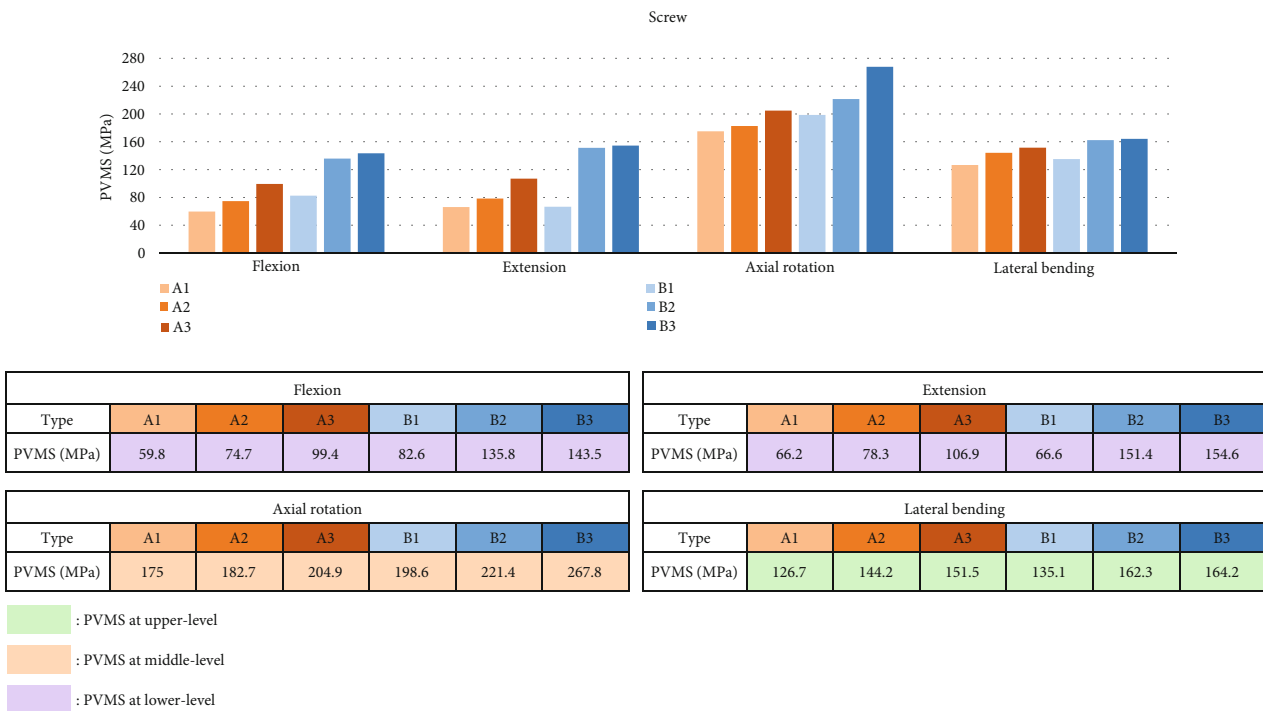


FIGURE 5: Peak von Mises stress measured at the screw.

Tsuchiya et al. reported that there was no case of screw loosening with multilevel fusion using iliac screw after 5 to 10 years of follow up [35]. In this study, we revealed biomechanical superiority of the use of iliac screws using 3-dimensional finite element method. Our results would be useful when deciding proper fusion level and instrumentation method in multilevel lumbar fusion surgery.

The risk of screw failure showed increasing pattern as the upper and lower levels extended in all motions (Figure 5). PVMS was identified at the neck of the screw in all motions and types, possibly due to the smaller diameter of the screw neck part (Figure 6). This was in accordance with the study conducted by Chen et al. [36]. The measured stress in all motion and types was less than the yield strength

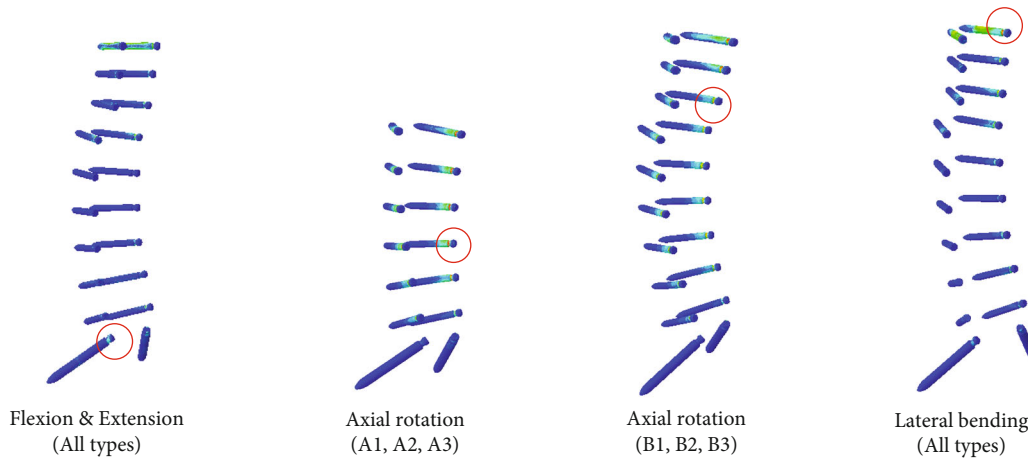


FIGURE 6: Location of peak von Mises stress at the screw.

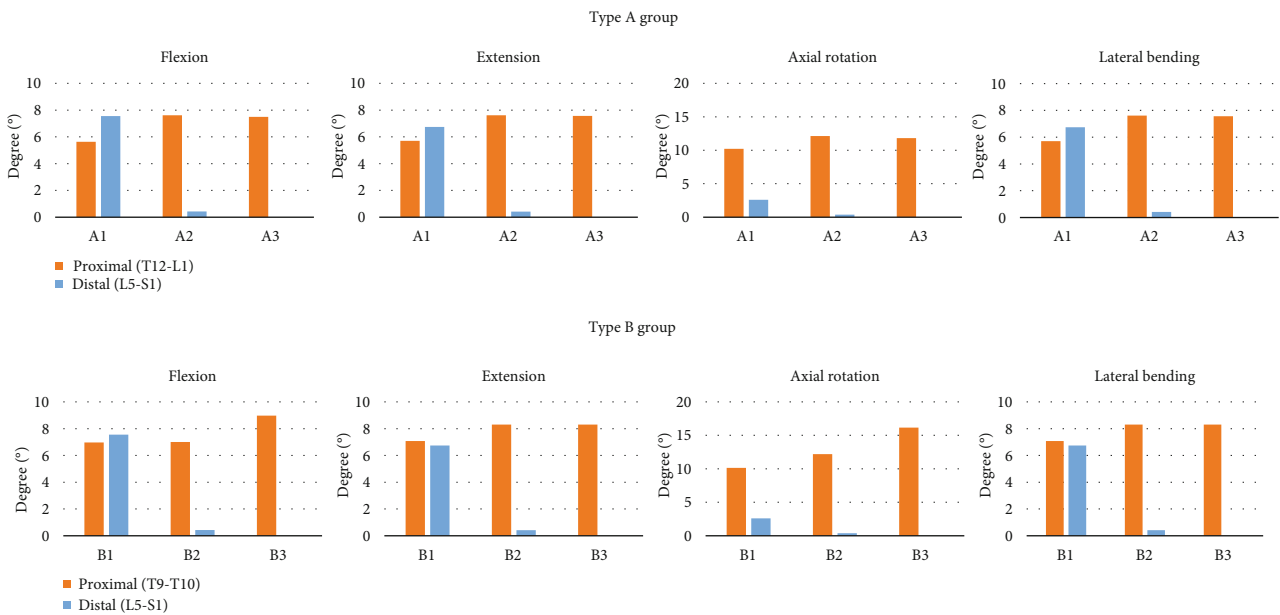


FIGURE 7: Range of motion at the proximal and distal junctions.

(880 MPa) of Grade 5 titanium (Ti-6Al-4V), implying the actual risk of screw breakage was not significantly high. Natarajan et al. indicated that the maximum von Mises stress occurs in the caudal portion of multilevel lumbar fusion [37]. In this study, we found that middle level and upper-level screws are also susceptible to failure in axial rotation and lateral bending motion, respectively.

Regarding lumbosacral junctional failure, we identified the superiority of fusion to the ilium compared with that to S1 using ROM analysis. Several previous studies have reported that extending the fusion to the ilium may prevent complications that arise from fusion to only S1 [16, 34, 35]. In this study, we found that multilevel fusion down to only S1 without iliac screws has micromotion, with an average of 0.4°, in the L5-S1 segment compared with fusion to the ilium with iliac screws (Figure 7).

The risk of proximal ASD increased as the fusion range increased to S1 and the ilium. The overall proximal ROM of type B group was similar or slightly higher, with an average of 13%, than that of type A group, a finding that was somewhat different from that of a previous clinical study [38]. Interestingly, type B3 had markedly higher (37%) proximal ROM than type A3 in axial rotation (Figure 7). A possible explanation may be that it is due to the difference in facet orientation between thoracic and lumbar vertebrae [39]. Because the facet orientation is parallel to the coronal plane, thoracic vertebrae have more rotation ability than lumbar vertebrae. When all the joints below T10 are fused, the T9-10 junction is more vulnerable in rotation motion owing to the high loading and rotation ability. Therefore, patient education regarding restricting excessive axial rotation movement would be helpful in T10-iliac fusion patients.

This study has several clinically relevant findings. Surgeons can determine the surgical outcome of patients according to various fusion levels. The risk of screw loosening and failure was numerically identified and can be applied to clinical practice. Furthermore, our results can be used as material for patient education.

Our study has limitations. First, we did not change the rod structure or material, such as the cobalt chrome rod or multiple-rod constructs. We considered the most used material and surgical technique to date to limit the variables. Further studies are needed to confirm the effect of the rod structure. Second, our model is based on a normal male individual; thus, it does not reflect the status of undercorrection or overcorrection and the poor bone quality observed in patients. Constructing a spine model based on a real patient with adult spinal deformity remains technically challenging. Further technical research is required to construct a real deformed spine model. In addition, the models in this study were considered as linear since we intended to see the trends between the models. We will apply the anisotropic properties of the bone in the future research. Finally, we assumed the screw-bone interface to be completely fused and fixed state and simplified the screw threads as previous finite element studies [40–45] since the size of the finite element model was large, and the screw loosening was thought to be a result of accumulated damage in the screw-bone interface for a long-term period. A more complex finite element model of a surface-to-surface contact with a coefficient friction between the screw-bone interface will be applied in the future study.

5. Conclusions

In multilevel lumbar fusion surgery for adult spinal deformity, adding iliac screws and increasing the fusion level to T10-iliac may lower the risk of screw loosening. In terms of screw failure and proximal ASD, however, T10-iliac fusion has a higher potential risk compared with other fusion types. These results will contribute for surgeons to provide adequate patient education regarding screw failure and proximal ASD, when performing multilevel lumbar fusion.

Data Availability

The datasets generated and/or analyzed during the current study are not publicly available due to the collaborative achievement related patent issue with collaborating research institute but are available from the corresponding author on reasonable request.

Conflicts of Interest

The authors declare that there is no conflict of interest regarding the publication of this article.

Authors' Contributions

Dong-Min Son and Soo-Bin Lee contributed equally to this work.

Acknowledgments

This research was supported by the Korea Institute for Advancement of Technology (KIAT) grant funded by the Korea Government Ministry of Trade Industry and Energy (MOTIE) (P092400007), and this research was supported by the Korea Medical Device Development Fund grant funded by the Korea Government (the Ministry of Science and ICT, the Ministry of Trade, Industry and Energy, the Ministry of Health & Welfare, and the Ministry of Food and Drug Safety) (KMDF_PR_20200901_0304).

References

- [1] H. J. Kim, J. H. Yang, D. G. Chang et al., "Adult spinal deformity: current concepts and decision-making strategies for management," *Asian Spine Journal*, vol. 14, no. 6, pp. 886–897, 2020.
- [2] J. A. Youssef, D. O. Orndorff, C. A. Patten et al., "Current status of adult spinal deformity," *Global Spine Journal*, vol. 3, no. 1, pp. 051–062, 2013.
- [3] F. Schwab, A. Dubey, L. Gamez et al., "Adult scoliosis: prevalence, SF-36, and nutritional parameters in an elderly volunteer population," *Spine*, vol. 30, no. 9, pp. 1082–1085, 2005.
- [4] C. P. Ames, J. K. Scheer, V. Lafage et al., "Adult spinal deformity: epidemiology, health impact, evaluation, and management," *Spine Deformity*, vol. 4, no. 4, pp. 310–322, 2016.
- [5] K. J. Cho, S. I. Suk, S. R. Park et al., "Short fusion versus long fusion for degenerative lumbar scoliosis," *European Spine Journal*, vol. 17, no. 5, pp. 650–656, 2008.
- [6] C. Scemama, F. Laouissat, K. Abelin-Genevois, and P. Roussouly, "Surgical treatment of thoraco-lumbar kyphosis (TLK) associated with low pelvic incidence," *European Spine Journal*, vol. 26, no. 8, pp. 2146–2152, 2017.
- [7] K. T. Kim, C. Y. Chan, S. H. Lee, D. S. Huh, and E. S. Son, "Surgical correction in patients with lumbar degenerative kyphosis who had low bone mineral density: an analysis of 40 patients with a minimum follow-up of two years," *Asian Spine Journal*, vol. 9, no. 1, pp. 65–74, 2015.
- [8] H. J. Kim, J. H. Yang, D. G. Chang et al., "Adult spinal deformity: a comprehensive review of current advances and future directions," *Asian Spine Journal*, vol. 16, no. 5, pp. 776–788, 2022.
- [9] J. K. Lee, S. J. Hyun, and K. J. Kim, "Reciprocal changes in the whole-body following realignment surgery in adult spinal deformity. Asian," *Asian Spine Journal*, 2022.
- [10] J. K. Biswas, M. Rana, A. Malas, S. Roy, S. Chatterjee, and S. Choudhury, "Effect of single and multilevel artificial intervertebral disc replacement in lumbar spine: a finite element study," *The International Journal of Artificial Organs*, vol. 45, no. 2, pp. 193–199, 2022.
- [11] K. H. Bridwell, C. C. Edwards, and L. G. Lenke, "The pros and cons to saving the L5-S1 motion segment in a long scoliosis fusion construct," *Spine*, vol. 28, no. 20, pp. S234–S242, 2003.
- [12] K. J. Cho, Y. T. Kim, S. H. Shin, and S. I. Suk, "Surgical treatment of adult degenerative scoliosis," *Asian Spine Journal*, vol. 8, no. 3, pp. 371–381, 2014.
- [13] B. S. Lee, K. M. Walsh, A. T. Healy et al., "Biomechanics of L5/S1 in long thoracolumbosacral constructs: a cadaveric study," *Global Spine Journal*, vol. 8, no. 6, pp. 607–614, 2018.

- [14] S. Bess, J. E. Harris, A. W. Turner et al., "The effect of posterior polyester tethers on the biomechanics of proximal junctional kyphosis: a finite element analysis," *Journal of Neurosurgery. Spine*, vol. 26, no. 1, pp. 125–133, 2017.
- [15] H. Mushlin, D. M. Brooks, J. Olexa et al., "A biomechanical investigation of the sacroiliac joint in the setting of lumbosacral fusion: impact of pelvic fixation versus sacroiliac joint fixation," *Journal of Neurosurgery. Spine*, vol. 31, no. 4, pp. 562–567, 2019.
- [16] T. R. Kuklo, K. H. Bridwell, S. J. Lewis et al., "Minimum 2-year analysis of sacropelvic fixation and L5-S1 fusion using S1 and iliac screws," *Spine*, vol. 26, no. 18, pp. 1976–1983, 2001.
- [17] S. Sohn, T. H. Park, C. K. Chung et al., "Biomechanical characterization of three iliac screw fixation techniques: a finite element study," *Journal of Clinical Neuroscience*, vol. 52, pp. 109–114, 2018.
- [18] M. A. Adams and P. Dolan, "Spine biomechanics," *Journal of Biomechanics*, vol. 38, no. 10, pp. 1972–1983, 2005.
- [19] A. T. Phillips, P. Pankaj, C. R. Howie, A. S. Usmani, and A. H. Simpson, "Finite element modelling of the pelvis: inclusion of muscular and ligamentous boundary conditions," *Medical Engineering & Physics*, vol. 29, no. 7, pp. 739–748, 2007.
- [20] M. Dalstra and R. Huiskes, "Load transfer across the pelvic bone," *Journal of Biomechanics*, vol. 28, no. 6, pp. 715–724, 1995.
- [21] N. S. Hakim and A. I. King, "A three dimensional finite element dynamic response analysis of a vertebra with experimental verification," *Journal of Biomechanics*, vol. 12, no. 4, pp. 277–292, 1979.
- [22] N. Kawahara, H. Murakami, A. Yoshida, J. Sakamoto, J. Oda, and K. Tomita, "Reconstruction after total sacrectomy using a new instrumentation technique: a biomechanical comparison," *Spine*, vol. 28, no. 14, pp. 1567–1572, 2003.
- [23] S. A. Shirazi-Adl, S. C. Shrivastava, and A. M. Ahmed, "Stress analysis of the lumbar disc-body unit in compression. A three-dimensional nonlinear finite element study," *Spine*, vol. 9, no. 2, pp. 120–134, 1984.
- [24] J. M. Buchowski, C. A. Kuhns, K. H. Bridwell, and L. G. Lenke, "Surgical management of posttraumatic thoracolumbar kyphosis," *The Spine Journal*, vol. 8, no. 4, pp. 666–677, 2008.
- [25] J. C. Liao, W. P. Chen, and H. Wang, "Treatment of thoracolumbar burst fractures by short-segment pedicle screw fixation using a combination of two additional pedicle screws and vertebroplasty at the level of the fracture: a finite element analysis," *BMC Musculoskeletal Disorders*, vol. 18, no. 1, 2017.
- [26] Y. Liang, Y. Cao, Z. Gong et al., "A finite element analysis on comparing the stability of different posterior fixation methods for thoracic total en bloc spondylectomy," *Journal of Orthopaedic Surgery and Research*, vol. 15, no. 1, p. 314, 2020.
- [27] C. B. Burns, K. Dua, N. A. Trasolini, D. E. Komatsu, and J. M. Barsi, "Biomechanical comparison of spinopelvic fixation constructs: iliac screw versus S2-alar-iliac screw," *Spine Deform*, vol. 4, no. 1, pp. 10–15, 2016.
- [28] J. Li, J. Shang, Y. Zhou, C. Li, and H. Liu, "Finite element analysis of a new pedicle screw-plate system for minimally invasive transforaminal lumbar interbody fusion," *PLoS One*, vol. 10, no. 12, article e0144637, 2015.
- [29] A. G. Patwardhan, R. M. Havey, K. P. Meade, B. Lee, and B. Dunlap, "A follower load increases the load-carrying capacity of the lumbar spine in compression," *Spine*, vol. 24, no. 10, pp. 1003–1009, 1999.
- [30] S. Oikonomidis, J. Greven, J. Bredow et al., "Biomechanical effects of posterior pedicle screw-based instrumentation using titanium versus carbon fiber reinforced PEEK in an osteoporotic spine human cadaver model," *Clinical Biomechanics*, vol. 80, article 105153, 2020.
- [31] S. Orita, S. Ohtori, Y. Eguchi et al., "Radiographic evaluation of monocortical versus tricortical purchase approaches in lumbosacral fixation with sacral pedicle screws: a prospective study of ninety consecutive patients," *Spine*, vol. 35, no. 22, pp. E1230–E1237, 2010.
- [32] L. Marie-Hardy, H. Pascal-Moussellard, A. Barnaba, R. Bonaccorsi, and C. Scemama, "Screw loosening in posterior spine fusion: prevalence and risk factors," *Global Spine Journal*, vol. 10, no. 5, pp. 598–602, 2020.
- [33] H. Z. Guo, Y. C. Tang, D. Q. Guo et al., "Pedicle screw fixation in single-level, double-level, or multilevel posterior lumbar fusion for osteoporotic spine: a retrospective study with a minimum 2-year follow-up," *World Neurosurgery*, vol. 140, pp. e121–e128, 2020.
- [34] T. Yasuda, T. Hasegawa, Y. Yamato et al., "Lumbosacral junctional failures after long spinal fusion for adult spinal deformity—which vertebra is the preferred distal instrumented vertebra?," *Spine Deformity*, vol. 4, no. 5, pp. 378–384, 2016.
- [35] K. Tsuchiya, K. H. Bridwell, T. R. Kuklo, L. G. Lenke, and C. Baldus, "Minimum 5-year analysis of L5-S1 fusion using sacropelvic fixation (bilateral S1 and iliac screws) for spinal deformity," *Spine*, vol. 31, no. 3, pp. 303–308, 2006.
- [36] C. S. Chen, W. J. Chen, C. K. Cheng, S. H. Jao, S. C. Chueh, and C. C. Wang, "Failure analysis of broken pedicle screws on spinal instrumentation," *Medical Engineering & Physics*, vol. 27, no. 6, pp. 487–496, 2005.
- [37] R. N. Natarajan, K. Watanabe, and K. Hasegawa, "Biomechanical analysis of a long-segment fusion in a lumbar spine—a finite element model study," *Journal of Biomechanical Engineering*, vol. 140, no. 9, 2018.
- [38] J. H. Kim, S. S. Kim, and S. I. Suk, "Incidence of proximal adjacent failure in adult lumbar deformity correction based on proximal fusion level," *Asian Spine Journal*, vol. 1, no. 1, pp. 19–26, 2007.
- [39] Y. Masharawi, B. Rothschild, G. Dar et al., "Facet orientation in the thoracolumbar spine: three-dimensional anatomic and biomechanical analysis," *Spine*, vol. 29, no. 16, pp. 1755–1763, 2004.
- [40] M. Xu, J. Yang, I. H. Lieberman, and R. Haddas, "Finite element method-based study of pedicle screw-bone connection in pullout test and physiological spinal loads," *Medical Engineering & Physics*, vol. 67, pp. 11–21, 2019.
- [41] L. La Barbera, C. Ottardi, and T. Villa, "Comparative analysis of international standards for the fatigue testing of posterior spinal fixation systems: the importance of preload in ISO 12189," *The Spine Journal*, vol. 15, no. 10, pp. 2290–2296, 2015.
- [42] L. La Barbera, F. Galbusera, H. J. Wilke, and T. Villa, "Pre-clinical evaluation of posterior spine stabilization devices: can the current standards represent basic everyday life activities?," *European Spine Journal*, vol. 25, no. 9, pp. 2909–2918, 2016.
- [43] J. W. Kwon, S. H. Bang, Y. W. Kwon et al., "Biomechanical comparison of the angle of inserted screws and the length of anterior cervical plate systems with allograft spacers," *Clinical Biomechanics*, vol. 76, article 105021, 2020.

- [44] J. W. Kwon, S. H. Bang, T. H. Park et al., “Biomechanical comparison of cervical discectomy/fusion model using allograft spacers between anterior and posterior fixation methods (lateral mass and pedicle screw),” *Clinical Biomechanics*, vol. 73, pp. 226–233, 2020.
- [45] S.-B. Lee, H.-M. Lee, T.-H. Park et al., “Biomechanical comparison of posterior fixation combinations with an allograft spacer between the lateral mass and pedicle screws,” *Applied Sciences*, vol. 10, no. 20, p. 7291, 2020.