

Research Article

High-Frequency Oscillatory Ventilation Combined with Volume Guarantee in a Neonatal Animal Model of Respiratory Distress Syndrome

Manuel Sánchez Luna,¹ Martín Santos González,² and Francisco Tendillo Cortijo²

¹Neonatology Division, Instituto de Investigación Sanitaria Gregorio Marañón, Hospital General Universitario “Gregorio Marañón”, C/ Dr. Esquerdo 46, 28007 Madrid, Spain

²Medical and Surgical Research Unit, Instituto de Investigación Sanitaria Puerta de Hierro Majadahonda, Hospital Universitario Puerta de Hierro Majadahonda, C/ Manuel de Falla 1, 28222 Madrid, Spain

Correspondence should be addressed to Manuel Sánchez Luna; msluna@salud.madrid.org

Received 10 April 2013; Revised 17 June 2013; Accepted 26 June 2013

Academic Editor: Frans B. Plötz

Copyright © 2013 Manuel Sánchez Luna et al. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Objective. To assess volume guarantee (VG) ventilation combined with high-frequency oscillatory ventilation (HFOV) strategy on PaCO₂ regulation in an experimental model of neonatal distress syndrome. **Methods.** Six 2-day-old piglets weighing 2.57 ± 0.26 kg were used for this interventional experimental study. Animals were ventilated during physiologic lung conditions and after depletion of lung surfactant by bronchoalveolar lavage (BAL). The effect of HFOV combined with VG on PaCO₂ was evaluated at different high-frequency expired tidal volume (V_{Thf}) at constant frequency (f_R) and mean airway pressure (mPaw). Fluctuations of the pressure (Δ Phf) around the mPaw and PaCO₂ were analyzed before and after lung surfactant depletion. **Results.** PaCO₂ levels were inversely proportional to V_{Thf}. In the physiological lung condition, an increase in V_{Thf} caused a significant decrease in PaCO₂ and an increase in Δ Phf. After BAL, PaCO₂ did not change as compared with pre-BAL situation as the V_{Thf} remained constant by the ventilator. **Conclusions.** In this animal model, using HFOV combined with VG, changes in the V_{Thf} settings induced significant modifications in PaCO₂. After changing the lung condition by depletion of surfactant, PaCO₂ remained unchanged, as the V_{Thf} setting was maintained constant by modifications in the Δ Phf done by the ventilator.

1. Introduction

High-frequency oscillatory ventilation (HFOV) is characterized by an effective gas exchange using tidal volumes equal to or less than the dead space volume [1] at supraphysiological frequencies. Carbon dioxide (CO₂) removal is mostly related to the tidal volume generated during high-frequency ventilation [2–5], and this high-frequency expired tidal volume (V_{Thf}) is known to be close to the airway dead space [6]. Also, the frequency (f_R) has a role in CO₂ removal [7] and has an independent effect on the distribution of the gas within the airways [8]. During HFOV, several mechanisms of gas exchange have been described, the combination of which is responsible for its ventilatory efficiency [9]. As HFOV uses a tidal volume lower or equal to the anatomical dead space,

it has been argued that the incidence of bronchopulmonary dysplasia (BPD) can be reduced [10]. Although other potential mechanisms have been described by which HFOV causes less ventilator-induced lung damage [11], the prevalence of BPD in preterm infants treated with HFOV is similar to those undergoing conventional ventilation [12].

V_{Thf} is crucial for CO₂ elimination and has a larger impact on CO₂ removal during HFOV in comparison to tidal volume during conventional mechanical ventilation. V_{Thf} is mostly generated by fluctuations of the pressure (Δ Phf) around the mean airway pressure (mPaw) and to the frequency f_R [13], but also the amount of V_{Thf} can be related to the endotracheal tube characteristics and compliance of the tubing as well as performance of the ventilator and lung conditions. Accordingly, large variations of V_{Thf} are

possible during HFOV, which in turn may cause unexpected variations of CO_2 removal [14].

VThf delivery depends on the ventilator characteristics, and although VThf monitoring is useful in daily practice, most of the ventilators providing HFOV do not display or measure the VThf [14–19]. However, in some new HFOV ventilators it is possible to adjust directly the VThf constant due to the volume guarantee (VG). VG is a well-documented volume target ventilation modality combined to synchronize conventional tidal ventilation [20], but this strategy has not been adequately evaluated during HFOV.

To assess the efficacy of adjusting VThf settings instead of $\Delta\text{P}_{\text{hf}}$ on PaCO_2 and the stability of VThf and PaCO_2 using VG ventilation during lung disease, an experimental study in a model of newborn piglets was conducted in which HFOV combined with VG was used before and after lung surfactant depression by bronchoalveolar lavage (BAL).

2. Materials and Methods

2.1. Animals. Six healthy 2-day-old Landrace-Large White piglets with a mean (\pm standard deviation, SD) body weight of 2.57 ± 0.26 kg were used. All animals were handled according to the Guide for the Care and Use of Laboratory Animals of the National Institutes of Health (<http://grants.nih.gov/grants/olaw/Guide-for-the-Care-and-Use-of-Laboratory-Animals.pdf>). Also, the ethics committee for animal care and use of the participating centers approved the study.

2.2. Anesthesia. General anesthesia was induced via facemask with 8% sevoflurane in oxygen. Then, a 24-gauge polyethylene catheter was placed into the ventrolateral auricular vein for continuous infusion of lactated Ringer’s solution (10 mL/kg/h) and the administration of drugs. Once an adequate level of anesthesia was achieved, an endotracheal tube (3 mm inner diameter) was placed and secured. Anesthesia was maintained with an intravenous (i.v.) constant infusion of propofol as needed, and intraoperative analgesia was achieved with i.v. morphine chlorhydrate (1 mg/kg).

2.3. Ventilation and Procedures. Animals were ventilated with HFOV combined with VG ventilation (Babylog VN500, Dräger, Lübeck, Germany). The following parameters were set: inspired oxygen fraction (FiO_2) of 0.3; continuous distending pressure of the airway (mean airway pressure (mPaw) of 10 cm H_2O ; tidal volume on HFOV (VThf) set as VG modality of 2 mL/kg; and respiratory frequency (f_R) of 10 Hz with a 1:1 inspiratory to expiratory ratio. The pressure swing around the mPaw (ΔP [$\Delta\text{P}_{\text{hf}}$]) and the carbon dioxide diffusion coefficient (DCO_2) calculated as $Vt^2 \times f_R$ (mL^2/sec) were obtained from the ventilator software (VentView 2.n software, Dräger, Lübeck, Germany).

Self-adhering parches were applied to the skin for ECG and heart rate (HR) recording. Pulse oximetry (SpO_2) was recorded continuously by placing a pulse oximeter on the paw, and rectal temperature (T^a) was also monitored and maintained between 36°C and 38°C by means of a total temperature management system. By surgical cut down, the

TABLE 1: Physiological variables at different VThf before and after surfactant depletion by BAL.

VThf/kg	HR (beats per min)	Mean BP (mmHg)	T^a ($^\circ\text{C}$)
2 mL/kg	160 ± 24	53 ± 10	37.2 ± 0.6
2.5 mL/kg	160 ± 17	53 ± 10	37.1 ± 0.8
3 mL/kg	149 ± 15	54 ± 11	37.1 ± 0.8
BAL	NA	NA	NA
3 mL/kg	137 ± 19	47 ± 8	36.0 ± 0.7

NA: not available.
Data as mean \pm SD.

endotracheal tube was sealed with a ribbon wrapped around the trachea to prevent any leak, and 18-gauge polyethylene catheter was inserted into right carotid artery. This access allowed for arterial blood sampling and continuous blood pressure measurement via a calibrated pressure transducer. T^a , SpO_2 , HR, and arterial blood pressure (BP) (referred to a zero level) were registered continuously on a cardiovascular monitor (PM8060 Vitarra, Dräger, Lübeck, Germany). Arterial blood was withdrawn anaerobically and immediately analyzed for pH, partial pressure of oxygen (PaO_2), partial pressure of carbon dioxide (PaCO_2), and arterial oxygen-hemoglobin saturation (SaO_2) (IL 1306 pH/Blood Gas Analyzer, Allied Instrumentation).

Following instrumentation and after a stabilization period of 15 min, baseline cardiorespiratory parameters and arterial blood samples were collected at a VThf of 2 mL/kg. Then, VThf was increased to 2.5 and 3 mL/kg at 15 min intervals. After each change in VThf, a 15 min period of stabilization was allowed before recording parameters. This was followed by BAL with 3 aliquots of 10 mL/kg isotonic saline solution warmed to body temperature [21, 22] to induce surfactant depletion mimicking neonatal respiratory distress syndrome.

To ensure adequate alveolar reexpansion, a sustained high-pressure recruitment maneuver using repeated 40 cm H_2O of pressure during 30 s was undertaken following BAL. A period of 30 min was determined to establish the surfactant-depleted situation, while the ventilator was set on HFOV with a VG of 3 mL/kg, and then arterial blood tests were done.

Data from the ventilator were exported through the standard USB connection.

2.4. Statistical Analysis. Statistical analysis was performed using SPSS 20.0 software program (IBM SPSS Statistics, Chicago, IL, USA). Continuous data were analyzed using an analysis of variance (ANOVA) for repeated measurement with the Bonferroni’s correction for multiple testing. Data are expressed as mean \pm SD. Statistical significance was set at $P < 0.05$.

3. Results

There were no differences in HR, arterial BP, and T^a among the animals during the study period (Table 1). The mean values of VThf for 2, 2.5, and 3 mL/kg were 5.0 ± 0.6 ,

TABLE 2: Physiological variables at different volumes guarantee before and after surfactant depletion by BAL.

VThf/kg	pH	PaO ₂ (mmHg)	PaCO ₂ (mmHg)	DCO ₂ (mL ² /sec)	ΔPhf (cm H ₂ O)
2 mL/kg	7.16 ± 0.064	78 ± 7	69 ± 11	247 ± 71	24 ± 6
2.5 mL/kg	7.22 ± 0.064	99 ± 11*	59 ± 12*	392 ± 109*	36 ± 8*
3 mL/kg	7.300 ± 0.074 ^{*,†}	107 ± 11*	51 ± 8*	569 ± 164 ^{*,†}	47 ± 12*
BAL	NA	NA	NA	NA	NA
3 mL/kg	7.24 ± 0.079	83 ± 14 ^{†,‡}	54 ± 10*	584 ± 141 ^{*,†}	50 ± 7*

NA: not applicable.

Data as mean ± SD.

* $P < 0.05$ (ANOVA) as compared to 2 mL/kg.

† $P < 0.05$ (ANOVA) as compared to 2.5 mL/kg.

‡ $P < 0.05$ (ANOVA) as compared to 3 mL/kg before BAL.

6.2 ± 0.9, and 7.6 ± 0.9 mL, respectively. The FiO₂ was maintained at 0.3 except during the BAL and the recruitment maneuvers (data not shown) when it was temporally increased as needed. Also, the frequency (10 Hz), mPaw (10 cm H₂O), and the inspiratory to expiratory ratio (1:1) were maintained constant throughout the study.

Mean values for all the animals of pH, PaO₂, PaCO₂, ΔP, and DCO₂ are shown in Table 2 at different VThf mL/kg during the physiological lung condition and after the BAL. HFOV with VG modality led to an increase in VThf, decrease in PaCO₂, and a significant increase in DCO₂ and measured ΔPhf (Table 2).

PaCO₂ was inversely proportional to VThf in all animals and remained constant after surfactant depletion, as compared with the pre-BAL situation (Figure 1). DCO₂ obtained from the ventilator increased with every increase in VThf during the physiological lung condition. After the BAL, DCO₂ remained constant (Figure 2) in all animals.

Measured ΔPhf increased in all the animals as VThf was increased in the lung physiological condition; after the BAL, ΔPhf increased in three animals, remained unchanged in one, and decreased in two, as the VThf remained constant in all of them (Figure 3); as well as the PaCO₂.

4. Discussion

In this study, using HFOV combined with VG in an animal model of neonatal distress syndrome during physiologic lung condition and after surfactant depletion, PaCO₂ was dependent on VThf. For every increase in VThf, an increase in ΔPhf and a significant decrease in PaCO₂ were observed. Using HFOV when the VG modality is not in use, fine-tuning changes of the ΔPhf and of the frequency of the ventilator have to be done to achieve the desired PaCO₂. In that situation, when ΔPhf is increased, VThf increases and more CO₂ is removed from the airways [6].

In our study, using HFOV combined with VG, for any increase in VThf there was a significant decrease in the PaCO₂, which was accompanied by an increase in ΔPhf, as this was done by the ventilator in response to the increase in VThf settings. We used a VThf of 2 to 3 mL/kg, as the expected dead space has been thought to be about 2.2 mL/kg in healthy awake neonates [23, 24] and the median delivered volume has been documented to be 2.4 mL/kg (range 1.0 to 3.6) [16].

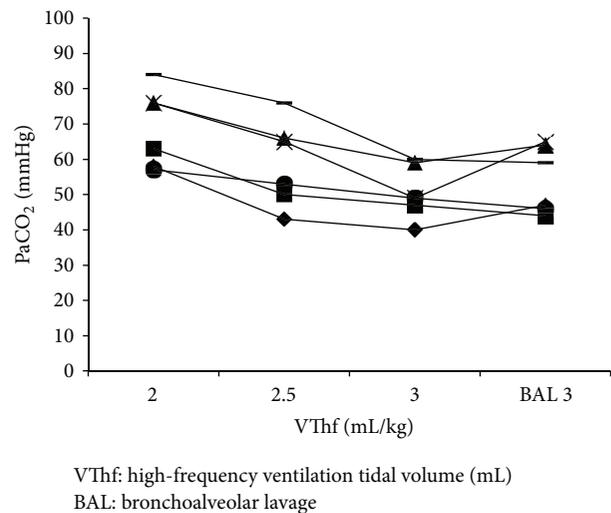


FIGURE 1: PaCO₂ determined at different VThf before and after surfactant depletion by bronchoalveolar lavage (BAL).

The exact mechanism for CO₂ removal when there is an increase of VThf during HFOV combined with VG is not fully understood, as the tidal bulk flow cannot explain it alone, and the VThf generated is lower or similar to the anatomical dead space, so a combination of several mechanisms is probably involved [25]. Also, although tidal volume has a greater effect on CO₂ elimination during HFOV than frequency [26], changes in the frequency induced changes in CO₂ removal, but probably by an independent mechanism [8]. When the VG modality is not in use in HFOV, as frequency is decreased, PaCO₂ decreases as well, and an increase in VThf may probably account for this finding [13], but some other mechanisms are probably involved, such as a better transmission of the pressure waves through the airways at lower frequencies [25]. It has been suggested that the optimal range of frequencies depends on both the body size and the intrinsic lung mechanics [27], and because finding this frequency is sometimes difficult, the use of a simple marker to guide settings for alveolar ventilation during HFOV will help on CO₂ removal. During HFOV, changes in the frequency will also modify ΔPhf to both proximal and distal lung compartments. Using HFOV without the VG modality, it was


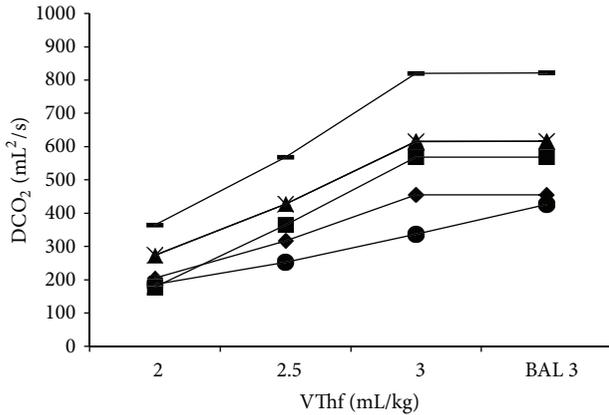


FIGURE 2: Carbon dioxide diffusion coefficient (DCO_2) calculated at different V_{Thf} before and after surfactant depletion by bronchoalveolar lavage (BAL). DCO_2 : carbon dioxide diffusion coefficient calculated as $Vt^2 \times f_R$ (mL^2/sec).

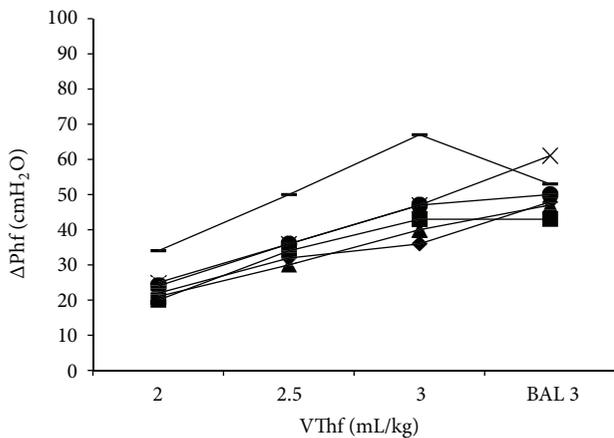

ΔPhf : pressures swing around the mean airway pressure (cmH_2O)
BAL: bronchoalveolar lavage

FIGURE 3: ΔPhf determined at different V_{Thf} before and after surfactant depletion by bronchoalveolar lavage (BAL).

recommended to set the highest frequency possible, while not compromising the V_{Thf} to prevent insufficient ventilation, to minimize ΔPhf , and to decrease barotrauma to the airways [15]. However, with the VG modality it is possible to combine the best frequency and modifying V_{Thf} , and this can be a preventive strategy to decrease lung damage.

We maintained a constant frequency as V_{Thf} was modified in order to assess better the isolated effect of the changes in V_{Thf} on $PaCO_2$, and a close relationship was found between both. So this VG modality will be more efficient not only at maintaining a more stable $PaCO_2$ but also to obtain fine modifications of the $PaCO_2$ and a better monitoring system during HFOV.

DCO_2 calculated as $Vt^2 \times f_R$ (mL^2/s) can be a marker of alveolar ventilation during HFOV. $PaCO_2$ increases as DCO_2 decreases, indicating alveolar hypoventilation [28]. In the present study, a clear effect of the changes of V_{Thf} on

DCO_2 was consistently observed in all animals during the physiological lung conditions. For any increase in V_{Thf} , there was a corresponding increase in DCO_2 . As the frequency was maintained unchanged, increases in DCO_2 were only related to V_{Thf} increases. Using HFOV with VG, any increase in V_{Thf} produced a significant increase in DCO_2 and a decrease in $PaCO_2$.

Also, and probably because of the use of a constant V_{Thf} and frequency when using the VG modality, after the surfactant lung-depleted situation, no changes in DCO_2 were found. In this respect, as may be expected, a constant and unchanged $PaCO_2$ was observed.

When the ventilator is using the VG modality during HFOV, the V_{Thf} is maintained constant, so the ventilator modifies ΔPhf to prevent any change in V_{Thf} . After the surfactant deficiency situation, the ventilator modified ΔPhf in all the animals to maintain V_{Thf} constant, and probably this is the main reason why $PaCO_2$ did not show a significant variation with any change in the lung condition. After the BAL, lung mechanics change fast, and an increase in ΔPhf was observed in three of the animals; in one there was no change, and in two there was a decrease. BAL produces a decrease in lung compliance [21, 22] that may affect V_{Thf} .

The effect of surfactant depletion on lung mechanics is variable, and because of the recruiting strategy used to prevent lung atelectasis, continuous changes are expected during and after the first minutes of lung lavage, so the use of the VG modality maintained the V_{Thf} stable throughout the study. In three of the animals the ventilator increased ΔPhf to maintain V_{Thf} , no change was observed in one animal and a decrease in ΔPhf was found in two, showing how V_{Thf} was maintained constant by the ventilator in any lung mechanics condition. This would add an advantage in the management of respiratory problems in the presence of a sudden change in lung mechanics. The ventilator, using the VG modality, will automatically modify ΔPhf to maintain a constant V_{Thf} , as it was demonstrated in this study, and because of that, significant variations of the $PaCO_2$ can probably be prevented. As it was expected, changes in lung mechanics produced by the surfactant depletion and the recruitment maneuvers were not uniform in all animals, mostly after the first minutes of the procedure, but as shown in the study, the ventilator using the VG modality maintains a constant V_{Thf} in any lung situation and in all the animals. After depletion of lung surfactant a low compliance situation is expected, but the effect of a decrease in the compliance on the V_{Thf} is variable. It has been demonstrated that modifications in respiratory compliance and mean airway pressure induced unexpected changes in V_{Thf} delivery, and also can vary depending on the type of ventilator. A decrease in V_{Thf} following an increase in lung compliance with the OHF 1 ventilator or an increase with the SensorMedics 3100^a has been reported [18]. High-frequency tidal volume is affected by the size of the endotracheal tube and patency of the airways, but is relatively insensitive to changes in lung tissue or chest wall mechanical properties [7]. This may partially explain why changes in ΔP were observed in only half of the animals after the BAL, as differing levels of compliance had little effect on delivered tidal volume related to the endotracheal tube size. The ventilatory frequency has

an important impact on airway reopening [29], but the effect of varying lung compliance on delivered tidal volume may be explained by the expected behavior of a simple harmonic (or oscillating) system. Modifying the frequency below or above the resonant frequency of a system, increasing compliance lowers impedance, resulting in greater flows for the same pressure, or the inertial effects dominate impedance, and compliance has little effect on its value. It has been demonstrated that changes in test lung compliance had a negligible effect on delivered tidal volume [30].

This situation can occur in a newborn with a severe respiratory distress syndrome (RDS) as the lung mechanics can change and the V_{Thf} sent from the ventilator can change when ΔP_{hf} instead of the V_{Thf} is set, so the use of the VG modality in those unstable conditions will probably prevent large variations in the $PaCO_2$. The variables exhibiting the greatest effect on the magnitude of delivered VT are frequency, ΔP , and endotracheal tube internal diameter [30].

In relation to a decrease of V_{Thf} seen with some ventilators when test lung compliance increased, this was mainly due to a decrease in ΔP [18], so that using a VG strategy with an automatic adjust of ΔP by the ventilator probably will prevent such variations in V_{Thf} when lung compliance changes.

The present findings should be interpreted taking into account some limitations of the study. The animal model does not reproduce the clinical condition of a newborn with severe RDS before and after giving surfactant. Because the aim of the study was to assess the effect of modifying directly the V_{Thf} instead of ΔP , a physiological situation was designed firstly in order to show this effect better. No previous studies have been published using the HFOV combined with VG showing this clear effect on arterial PCO_2 after an increase in the V_{Thf} during HFOV; therefore, a physiologic lung condition and the response of the $PaCO_2$ after modifications in the V_{Thf} were designed. As the effect of BAL on lung mechanics of the animals was not homogeneous, we also assessed how the ventilator would maintain constant V_{Thf} modifying or not ΔP after BAL depending on the change of the lung mechanics. Also, the BAL effect on lung mechanics is variable among the animals as a recruitment strategy was used immediately after the lavage to prevent a severe atelectasis.

5. Conclusions

The use of HFOV combined with VG ventilation in this newborn animal model of surfactant deficiency allowed for setting the V_{Thf} instead of ΔP_{hf} to modify CO_2 removal from the lung. A significant decrease in $PaCO_2$ with any increase in V_{Thf} was found. For any change of the V_{Thf} setting, the ventilator modified ΔP_{hf} to maintain the V_{Thf} . After BAL, the ventilator modified ΔP_{hf} to maintain a constant V_{Thf} as needed, and $PaCO_2$ remained unchanged compared to the pre-surfactant depletion condition.

List of Abbreviations

HFOV: High-frequency oscillatory ventilation
 V_{Thf} : High-frequency expired tidal volume
 CO_2 : Carbon dioxide

f_R : Frequency
 ΔP_{hf} : Delta pressure
mPaw: Mean airway pressure
VG: Volume guarantee
BAL: Bronchoalveolar lavage
SD: Standard deviation
i.v.: Intravenous
 FiO_2 : Inspired oxygen fraction
 DCO_2 : Carbon dioxide diffusion coefficient
HR: Heart rate
 SpO_2 : Pulse oximetry
 T^a : Rectal temperature
BP: Blood pressure
 PaO_2 : Partial arterial oxygen pressure
 $PaCO_2$: Partial carbon dioxide pressure
 SaO_2 : Arterial oxyhemoglobin saturation
RDS: Respiratory distress syndrome.

Conflict of Interests

Manuel Sánchez Luna declares receiving advisory board consulting fees from Dräger. The remaining authors declare that they have no competing interests.

Acknowledgments

The authors thank Dräger Medical GmbH for providing the Babylog VN500 for the present study and Marta Pulido, M.D., for editing the paper and Jaques Belik for reviewing it.

References

- [1] A. S. Slutsky, J. M. Drazen, and R. H. Ingram Jr., "Effective pulmonary ventilation with small-volume oscillations at high frequency," *Science*, vol. 209, no. 4456, pp. 609–611, 1980.
- [2] A. S. Slutsky, "Gas mixing by cardiogenic oscillations: a theoretical quantitative analysis," *Journal of Applied Physiology Respiratory Environmental and Exercise Physiology*, vol. 51, no. 5, pp. 1287–1293, 1981.
- [3] T. H. Rossing, A. S. Slutsky, J. L. Lehr, P. A. Drinker, R. Kamm, and J. M. Drazen, "Tidal volume and frequency dependence of carbon dioxide elimination by high-frequency ventilation," *New England Journal of Medicine*, vol. 305, no. 23, pp. 1375–1379, 1981.
- [4] M. J. Jaeger, U. H. Kurzweg, and M. J. Banner, "Transport of gases in high-frequency ventilation," *Critical Care Medicine*, vol. 12, no. 9, pp. 708–710, 1984.
- [5] D. R. Spahn, R. Leuthold, E. R. Schmid, and P. F. Niederer, "Significance of bulk convection during high-frequency oscillation," *Respiration Physiology*, vol. 84, no. 1, pp. 1–11, 1991.
- [6] D. Isabey, A. Harf, and H. K. Chang, "Alveolar ventilation during high-frequency oscillation: core dead space concept," *Journal of Applied Physiology Respiratory Environmental and Exercise Physiology*, vol. 56, no. 3, pp. 700–707, 1984.
- [7] J. J. Fredberg, G. M. Glass, B. R. Boynton, and I. D. Frantz III, "Factors influencing mechanical performance of neonatal high-frequency ventilators," *Journal of Applied Physiology*, vol. 62, no. 6, pp. 2485–2490, 1987.
- [8] D. P. Schuster, R. Karsch, and K. P. Cronin, "Gas transport during different modes of high-frequency ventilation," *Critical Care Medicine*, vol. 14, no. 1, pp. 5–11, 1986.

- [9] A. S. Slutsky and J. M. Drazen, "Ventilation with small tidal volumes," *New England Journal of Medicine*, vol. 347, no. 9, pp. 630–631, 2002.
- [10] R. H. Clark, D. R. Gerstmann, D. M. Null Jr., and R. A. DeLemos, "Prospective randomized comparison of high-frequency oscillatory and conventional ventilation in respiratory distress syndrome," *Pediatrics*, vol. 89, no. 1, pp. 5–12, 1992.
- [11] V. K. Rehan, J. Fong, R. Lee et al., "Mechanism of reduced lung injury by high-frequency nasal ventilation in a preterm lamb model of neonatal chronic lung disease," *Pediatric Research*, vol. 70, no. 5, pp. 462–466, 2011.
- [12] F. Cools, L. M. Askie, M. Offringa et al., "Elective high-frequency oscillatory versus conventional ventilation in preterm infants: a systematic review and meta-analysis of individual patients' data," *The Lancet*, vol. 375, no. 9731, pp. 2082–2091, 2010.
- [13] V. Chan, A. Greenough, and A. D. Milner, "The effect of frequency and mean airway pressure on volume delivery during high-frequency oscillation," *Pediatric pulmonology*, vol. 15, no. 3, pp. 183–186, 1993.
- [14] M. Zimová-Herknerová and R. Plavka, "Expired tidal volumes measured by hot-wire anemometer during high-frequency oscillation in preterm infants," *Pediatric Pulmonology*, vol. 41, no. 5, pp. 428–433, 2006.
- [15] C. C. Dos Santos and A. S. Slutsky, "Overview of high-frequency ventilation modes, clinical rationale, and gas transport mechanisms," *Respiratory Care Clinics of North America*, vol. 7, no. 4, pp. 549–575, 2001.
- [16] G. Dimitriou, A. Greenough, V. Kavvadia, B. Laubscher, and A. D. Milner, "Volume delivery during high frequency oscillation," *Archives of Disease in Childhood: Fetal and Neonatal Edition*, vol. 78, no. 2, pp. F148–F150, 1998.
- [17] J. A. Leipälä, S. Iwasaki, A. Milner, and A. Greenough, "Accuracy of the volume and pressure displays of high frequency oscillators," *Archives of Disease in Childhood: Fetal and Neonatal Edition*, vol. 89, no. 2, pp. F174–F176, 2004.
- [18] P. Jouviet, P. Hubert, D. Isabey et al., "Assessment of high-frequency neonatal ventilator performances," *Intensive Care Medicine*, vol. 23, no. 2, pp. 208–213, 1997.
- [19] G. Vento, M. Tana, C. Tirone et al., "Unexpected effect of recruitment procedure on lung volume measured by respiratory inductive plethysmography (RIP) during high frequency oscillatory ventilation (HFOV) in preterm neonates with respiratory distress syndrome (RDS)," *Journal of Maternal-Fetal and Neonatal Medicine*, vol. 24, no. 1, pp. 159–162, 2011.
- [20] C. Klingenberg, K. I. Wheeler, P. G. Davis, and C. J. Morley, "A practical guide to neonatal volume guarantee ventilation," *Journal of Perinatology*, vol. 31, pp. 575–585, 2011.
- [21] B. Lachmann, B. Robertson, and J. Vogel, "In vivo lung lavage as an experimental model of the respiratory distress syndrome," *Acta Anaesthesiologica Scandinavica*, vol. 24, no. 3, pp. 231–236, 1980.
- [22] C. Rosenthal, C. Caronia, C. Quinn, N. Lugo, and M. Sagy, "A comparison among animal models of acute lung injury," *Critical Care Medicine*, vol. 26, no. 5, pp. 912–916, 1998.
- [23] D. Lagneaux, C. Mossay, F. Geubelle, and G. Christiaens, "Alveolar data in healthy, awake neonates during spontaneous ventilation: a preliminary investigation," *Pediatric Pulmonology*, vol. 5, no. 4, pp. 225–231, 1988.
- [24] A. H. Numa and C. J. L. Newth, "Anatomic dead space in infants and children," *Journal of Applied Physiology*, vol. 80, no. 5, pp. 1485–1489, 1996.
- [25] J. J. Pillow, "High-frequency oscillatory ventilation: mechanisms of gas exchange and lung mechanics," *Critical Care Medicine*, vol. 33, no. 3, pp. S135–S141, 2005.
- [26] H. Korvenranta, W. A. Carlo, D. A. Goldthwait Jr., and A. A. Fanaroff, "Carbon dioxide elimination during high-frequency jet ventilation," *Journal of Pediatrics*, vol. 111, no. 1, pp. 107–113, 1987.
- [27] B. R. Boynton, M. D. Hammond, J. J. Fredberg, B. G. Buckley, D. Villanueva, and I. D. Frantz III, "Gas exchange in healthy rabbits during high-frequency oscillatory ventilation," *Journal of Applied Physiology*, vol. 66, no. 3, pp. 1343–1351, 1989.
- [28] J. G. Venegas and J. J. Fredberg, "Understanding the pressure cost of ventilation: why does high-frequency ventilation work?" *Critical Care Medicine*, vol. 22, no. 9, pp. S49–S57, 1994.
- [29] K. Bauer and C. Brücker, "The role of ventilation frequency in airway reopening," *Journal of Biomechanics*, vol. 42, no. 8, pp. 1108–1113, 2009.
- [30] D. N. Hager, H. E. Fessler, D. W. Kaczka et al., "Tidal volume delivery during high-frequency oscillatory ventilation in adults with acute respiratory distress syndrome," *Critical Care Medicine*, vol. 35, no. 6, pp. 1522–1529, 2007.



Hindawi

Submit your manuscripts at
<http://www.hindawi.com>

