


Supplement Figure 1

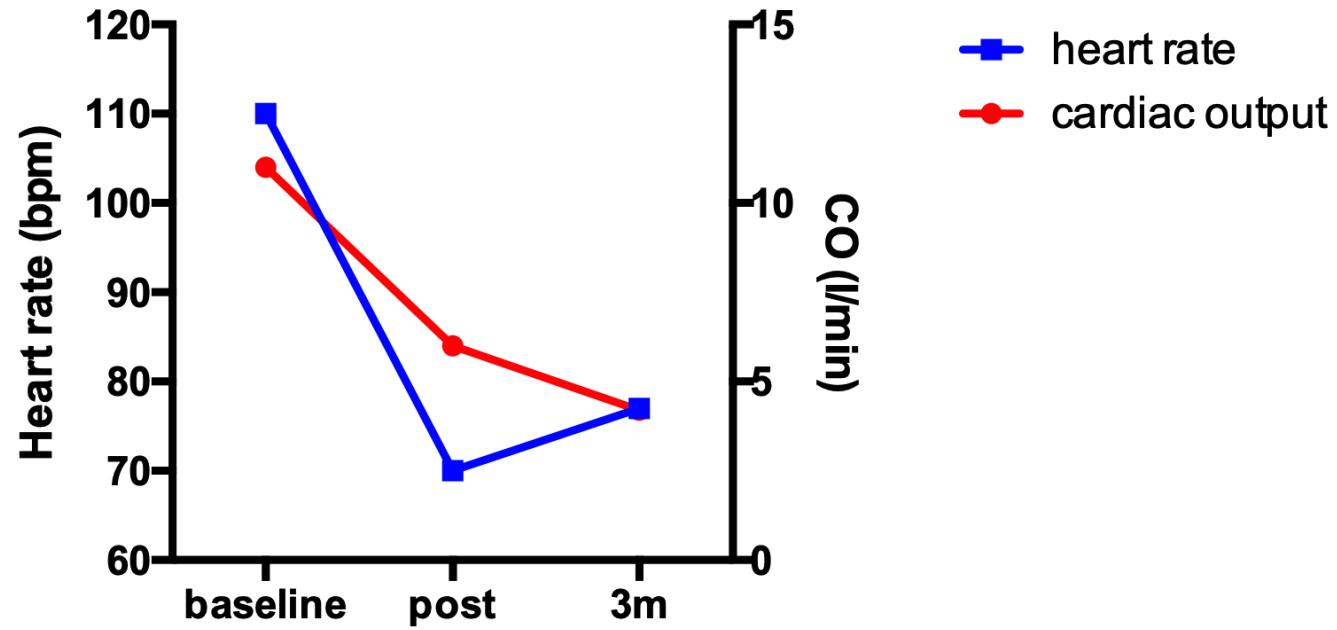

Supplement Figure 1: Heart rate (bpm) and cardiac output (CO) over 3 time course of 3 months. Elevated bpm and CO prior to treatment. Both parameters normalized two days (post) and 3 months (3m) after the occlusion of the RAVF utilizing Amplatzer Vascular Plug (AVP) Device II. Concordantly, the patient's physical capacity improved.