




Table S9. Spectral data of compound 9

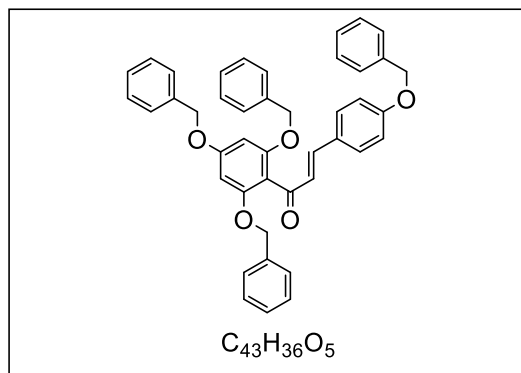

UV

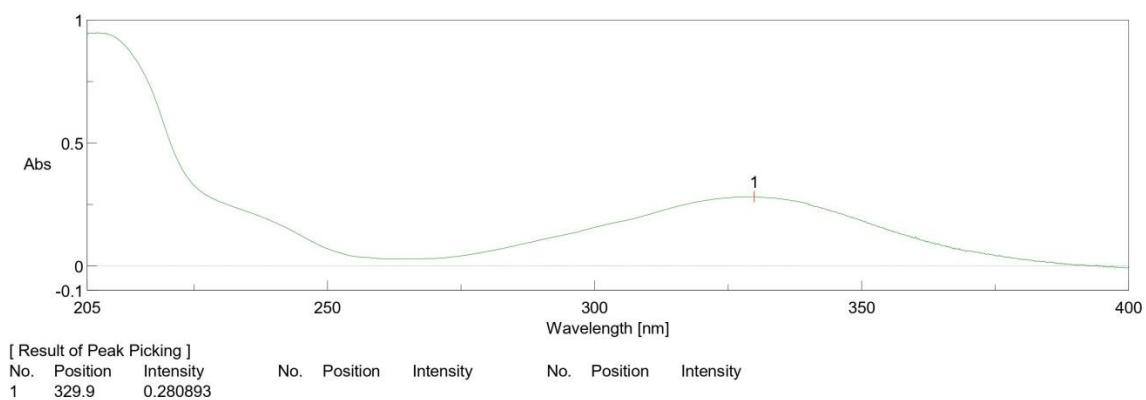

IR

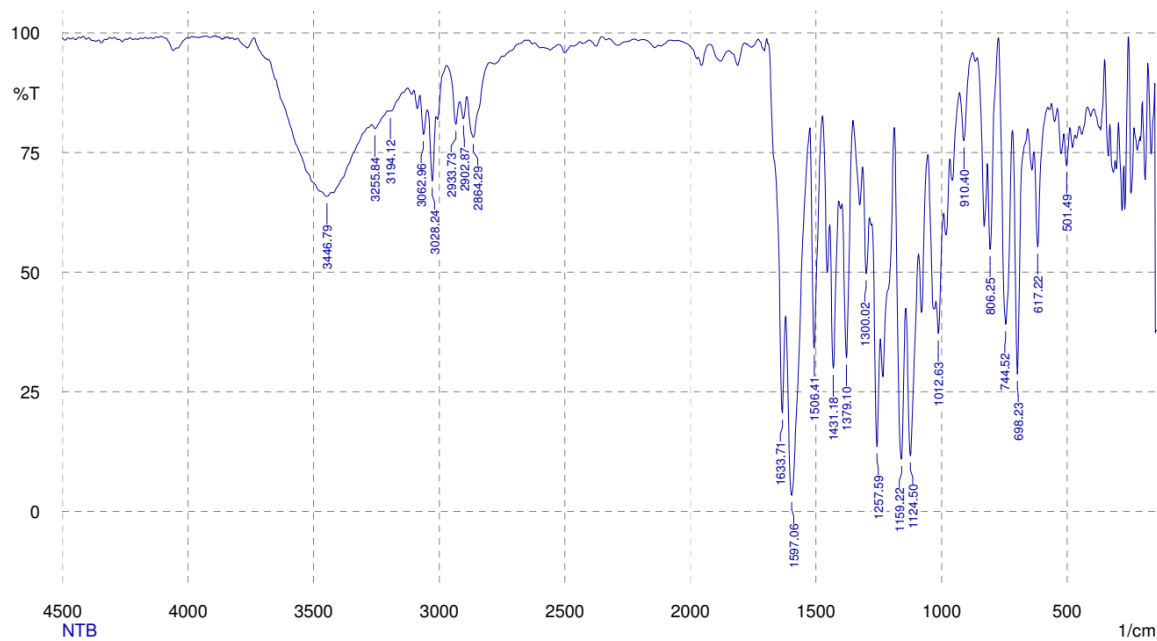


HR-MS

Qualitative Analysis Report

Data File	NTBc.d	Sample Name	NTBc
Sample Type	Sample	Position	P1-A9
Instrument Name	Instrument 1	User Name	
Acq Method	Cot ngan - MSMS_Pos.m	Acquired Time	01/07/2021 3:45:27 PM
IRM Calibration Status	Success	DA Method	COTNGAN.M.m
Comment			
Sample Group		Info.	
Stream Name	LC 1	Acquisition SW Version	6200 series TOF/6500 series Q-TOF B.06.01 (B6172 SP1)

User Chromatograms

Fragmentor Voltage 140 Collision Energy 0 Ionization Mode ESI

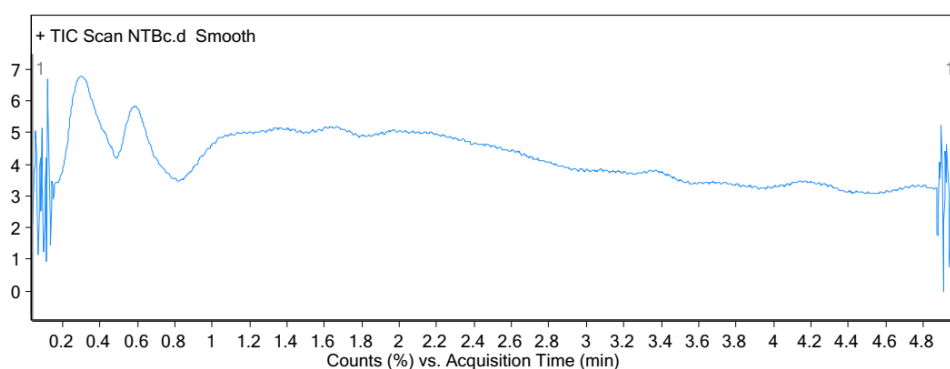

Agilent Technologies


Page 1 of 4

Printed at 12:29 AM on 2-Jul-2021


Qualitative Analysis Report

User Spectra

Fragmentor Voltage 140 Collision Energy 0 Ionization Mode ESI

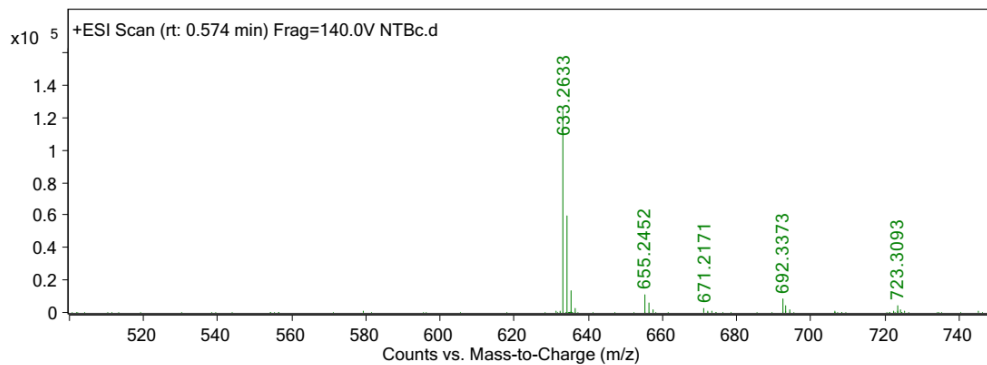


Sample Name	NTBc	Position	P1-A9	Instrument Name	Instrument 1
User Name		Inj Vol	2	InjPosition	
Sample Type	Sample	IRM Calibration Status	Success	Data Filename	NTBc.d
ACQ Method	Cot ngan - MSMS_Pos.m	Comment		Acquired Time	01/07/2021 3:45:27 PM

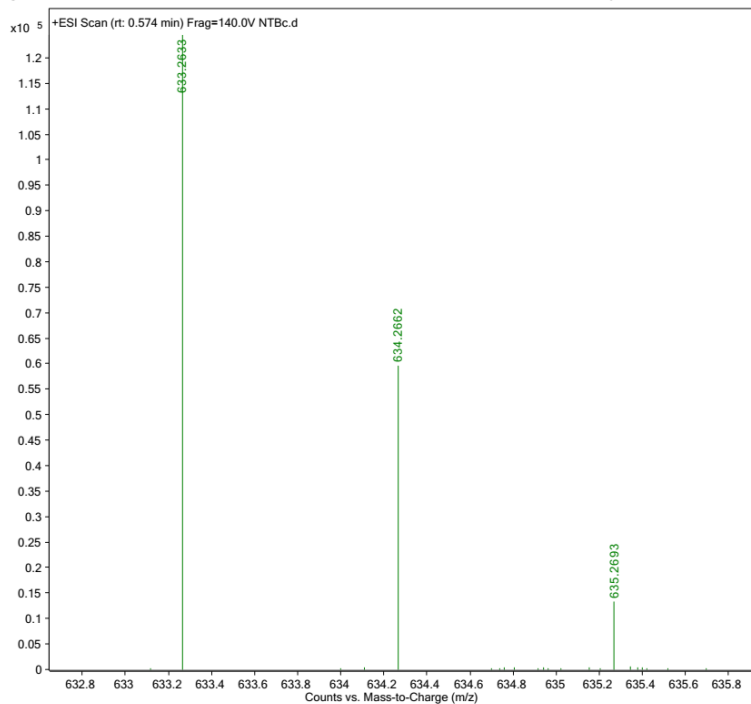

¹H-NMR

NTB-DMSO-1H

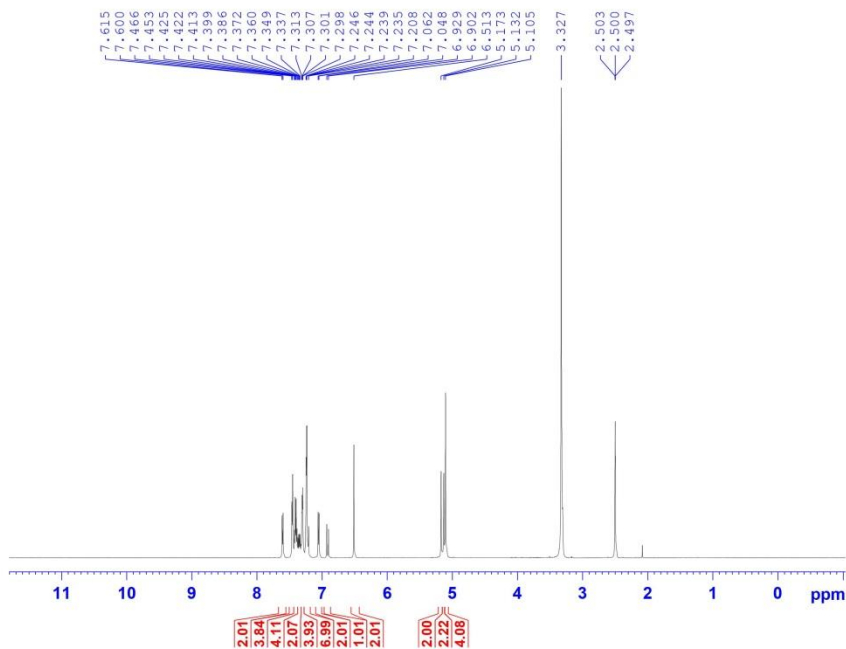


Current Data Parameters
NAME 110HUAN_NTB
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210204
Time 11.29 h
INSTRUM AvanceNEO 600MHz
PROBHD Z114607_0862 (1
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 11904.762 Hz
FIDRES 0.363304 Hz
AQ 2.7525120 sec
RG 101
DM 42.000 usec
DE 8.79 usec
TE 300.0 K
D1 1.00000000 sec
TDO 1
SFO1 600.3637072 MHz
NUC1 1H
FO 3.33 usec
P1 10.00 usec
PLM1 27.03700066 W


F2 - Processing parameters
SI 65536
SF 600.3600048 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

NTB-DMSO-1H

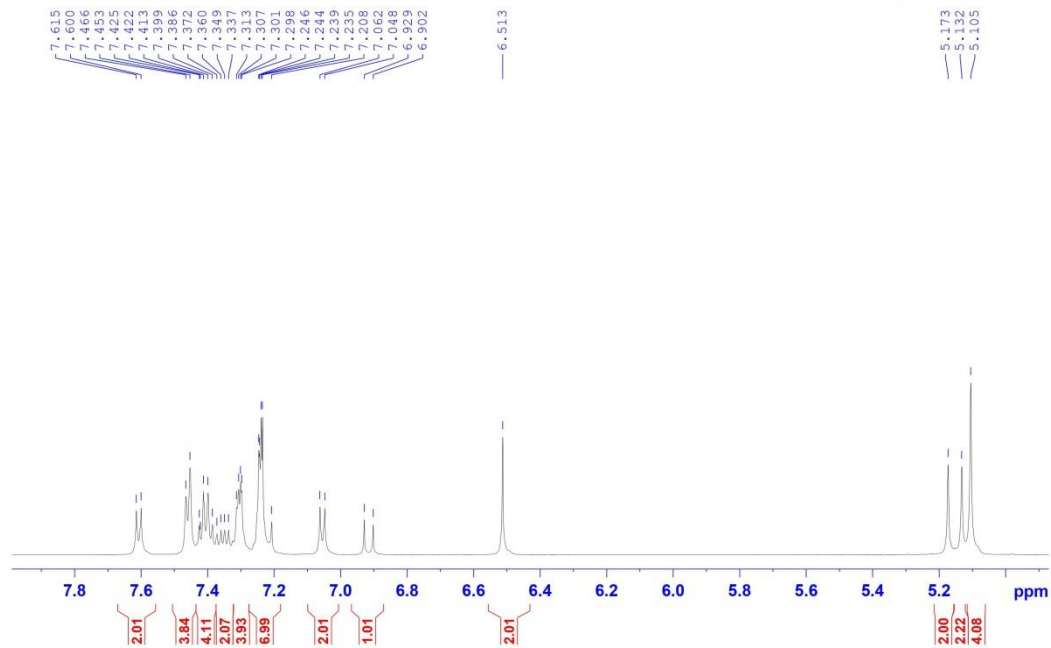

^{13}C -NMR

NTB-DMSO-C13CPD

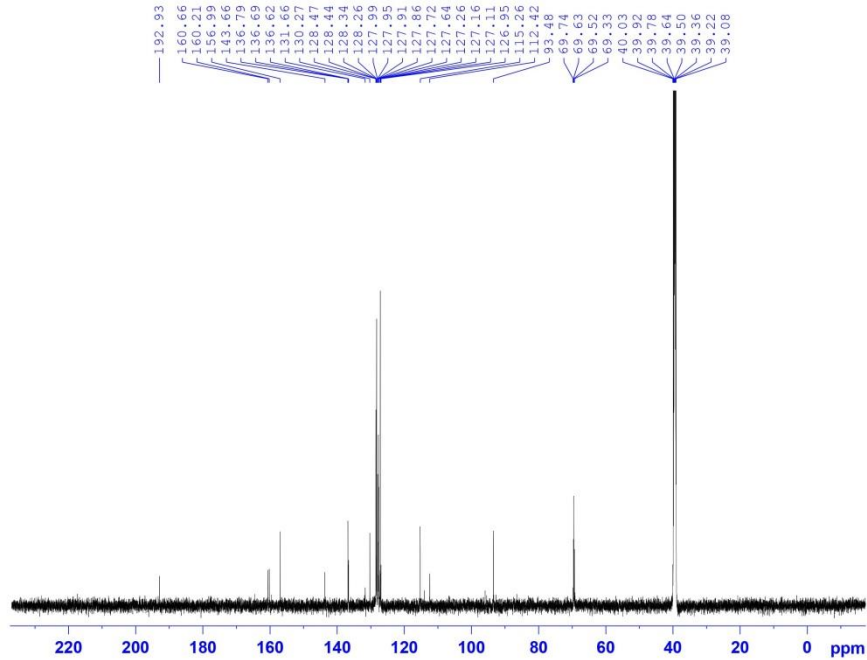

NTB-DMSO-C13CPD

